

## Relative efficacy of three Ni-Ti file systems used by undergraduates

Hyeon-Cheol Kim, Jeong-Kil Park, Bock Hur\*

*Department of Conservative Dentistry, College of Dentistry, Pusan National University*

### ABSTRACT

The purpose of this study was to compare and evaluate the shaping ability of the three different Ni-Ti file systems used by undergraduate students.

Fifty undergraduate students prepared 150 simulated curved root canals in resin blocks with three Ni-Ti file systems - ProFile® (PF), Manual ProTaper® (MPT), Rotary ProTaper® (RPT). Every student prepared 3 simulated root canals with each system respectively. After root canal preparation, the Ni-Ti files were evaluated for distortion or breakage. Assessments were made according to the presence of various types of canal aberrations. The pre- and post-instrumented canal images were attained and superimposed. The instrumented root canal width were measured and calculated for the net transportation (deviation) and the centering ratio.

Under the condition of this study, both ProTaper® systems allowed significantly more removal of root canal wall than the ProFile® system. In the important other aspects such as the centering ratio, there was no significant differences between the systems. Novice dental students were able to prepare curved root canals with any kinds of Ni-Ti file systems with little aberration and great conservation of tooth structure. Students want to learn effective methods and at the same time simple rotary procedures. The rotary ProTaper® systems were one of the most compatible to these students from the point of view of cutting ability. The ProFile® system was also compatible in safe and gentle shaping. [J Kor Acad Cons Dent 30(1):38-48, 2005]

**Key words** : Undergraduates, Ni-Ti file system, Shaping ability, Centering ratio

- received 2004. 12. 24, accepted 2004. 12. 30 -

### I. Introduction

Three dimensional root canal shaping and its hermetic obturation are the major elements determine the predictability of successful endodontics. In order to facilitate the irrigation process during

the root canal preparation, adequate root canal shaping is also considered as a key requirement.

Conventional endodontic files are manufactured from stainless-steel, and these files have been used successfully with the concept of step-back preparation technique. Since the end of 1980's, files made of nickel-titanium (Ni-Ti) have become available. Although hand files made of Ni-Ti are available, engine-driven rotary Ni-Ti instruments and crown-down techniques have revolutionized root canal preparations and are gaining in popularity<sup>1)</sup>. Numerous studies have shown that Ni-Ti rotary instruments can effectively produce a well-tapered

---

\* Corresponding author: **Bock Hur**

Department of Conservative Dentistry,  
College of Dentistry, Pusan National University  
1-10 Ami-dong, Seo-gu, Busan, 602-739, Korea  
Tel : 82-51-240-7454  
E-mail : bhur@pusan.ac.kr

root canal form sufficient for obturation, with minimal risk of transporting the original canal<sup>12-5</sup>.

Many Ni-Ti file systems have been introduced to the market. Most of these Ni-Ti file systems - e.g. ProFile<sup>®</sup> (Dentsply Maillefer, Ballaigues, Switzerland), K3<sup>™</sup> (SybronEndo, Glendora, France), Hero642<sup>®</sup> (Micromega, Besancon, France) - have a constant tapered shaft design, while these have various rake angles and radial land respectively<sup>6-8</sup>. The recently developed ProTaper<sup>®</sup> (Dentsply Maillefer, Ballaigues, Switzerland) has a progressive tapered shaft design<sup>9,10</sup>. They are manufactured in different sizes from ISO standardization and each instrument has a variable taper. ProTaper<sup>®</sup> has two types on the market, the manual ProTaper<sup>®</sup> and rotary ProTaper<sup>®</sup>. The ProFile<sup>®</sup> system can be categorized as a passive instrument, while the ProTaper<sup>®</sup> (manual and rotary) system works with an active cutting motion<sup>10</sup>.

There have been many studies suggesting that rotary preparation with Ni-Ti instruments has many advantages over hand preparation with conventional stainless-steel instruments, both for experienced and for inexperienced operators<sup>5,11,12</sup>. However, few studies<sup>13-15</sup> have addressed the use of Ni-Ti file systems by undergraduates. Currently no curriculum from any school adequately prepares its students to understand and practically apply the Ni-Ti file systems<sup>16,17</sup>. If the Ni-Ti preparation technique is included in an undergraduate curriculum, the arising question is which system would be the most effective.

The purpose of this study was to compare and evaluate the shaping abilities of three Ni-Ti file systems (ProFile<sup>®</sup>, manual ProTaper<sup>®</sup>, rotary ProTaper<sup>®</sup>) used by undergraduate students.

## II. Materials and Methods

Fifty senior undergraduate students at the Dental College of Pusan National University (Busan, Korea) with no practical experience using Ni-Ti file systems in root canal preparation participated in this study. The regular curriculum instruction in root canal shaping procedures consists of six hours of lecture and eight hours of

model (extracted tooth) exercises with stainless-steel files. This was the entirety of the students exposure to the procedures. In addition to the lectures on basic and practical endodontics of the regular curriculum, the students received two hours of lecture and watched video about the three systems used in this study. Respective instrumentation procedures were demonstrated before the start of the experiment.

The students prepared 150 simulated curved root canals in resin blocks (Endo Training Bloc; Dentsply Maillefer, Ballaigues, Switzerland) using the three Ni-Ti file systems - ProFile<sup>®</sup> (PF), manual ProTaper<sup>®</sup> (MPT), rotary ProTaper<sup>®</sup> (RPT). Every student prepared three simulated root canals with each system.

### 1. Specimen and instrumentation

#### 1-1. Simulated root canals

The simulated root canal blocks used in this study had a vertical length of 14 mm straightly from the level of apical foramen to orifice level and the root canals had about 16 mm of working length and about 40° curvature angle. Aqueous red ink was injected into the canals to enhance the image contrast. These resin blocks were scanned in a reproducible position with a scanner (Scanjet<sup>®</sup>; C8510A, Hewlett-Packard, California, USA), and then the image data was stored in a personal computer.

#### 1-2. Instrumentation

All Ni-Ti files used in this study were new ones. These files were used in the manner of manufacturer's recommendation. The MPT was operated by hand. Both the PF and RPT were operated by an electric motor (Tecnika<sup>®</sup>; ATR, Pistola, Italy) set at a speed of 300 rpm and torque of 30 (Tecnika motor setting value) in a 16:1 reduction handpiece. These settings were within the range suggested by the manufacturer. The instrumentation sequence of each system is summarized in Table 1. During the procedures, all simulated canals were verified the patency, then irrigated and lubricated with the RC-prep<sup>®</sup> (Stone Phar-

maceuticals, Philadelphia, USA) step-by-step.

## 2. Measurement techniques

### 2-1. Instrument distortion or breakage

After root canal preparation, the Ni-Ti files were evaluated for distortion or breakage using a microscope at 25× magnification (OPMI® pico Surgical Microscope; Carl Zeiss, Oberkochen, Germany).

### 2-2. Aberrations

After root canal preparation was completed, aqueous methylene blue solution was injected into the enlarged canals. The resin blocks were scanned again in a reproducible position as previously described. The scanned images were assessed on a 17 inch TFT-LCD monitor (SyncMaster® CX701N; Samsung, Suwon, Korea) using Adobe® Photoshop ver.7.0 (Adobe, San Jose, California, USA). Assessments were made according to the presence of various types of canal aberrations such as apical zip, elbow and ledge.

### 2-3. Preparation time

Canal preparation time was recorded in minutes and seconds by each student. The recorded time included the time for irrigation, changing instruments and recapitulation.

2-4. Instrumented canal width, net transportation, and centering ratio

Using Adobe® Photoshop software, the pre- and post-instrumented canal images were superimposed on one another and were observed at a magnification of 156 times. Measurements were taken horizontally at three different levels (1, 3, and 5 mm) from the level of apical foramen. The levels are selected for evaluation of terminal point, mid-point, and beginning point of root canal curvature.

Widths were measured linearly from the pre-instrumented point to the post-instrumented wall inwardly and outwardly at each level. These values were used to calculate the instrumented canal width and post-instrumented canal diameter.

The net transportation (deviation) was determined from the discrepancy between outward and inward-instrumented width (Figure 1). The direction of canal transportation was acquired by the negative or positive value. A negative value indicates an inward deviation.

The centering ratio was computed to evaluate the movement of root canal's center after preparation. The ratio was calculated using the following method: the absolute value of net transportation divided by whole width of the post-instrumented canal. The centering ratio is a measure of the ability of the instrument to stay

**Table 1.** The instrumentation procedures of the Ni-Ti file systems

ProFile®	ProTaper® (manual and rotary)
OS3 to resistance	Explorer canal with #10 followed by #15
OS2 to resistance	S1 to flare coronal until the depth of #15
.06 #25 to resistance	SX for more coronal flaring
.06 #20 to resistance	Measure working length
.04 #25 to resistance	S1 to working length
Measure working length	S2 to working length
.04 #20 to working length	F1 to working length
.04 #25 to working length	Apical gauging with #20
.06 #20 to working length	F2 to working length
Apical gauging with #25	Apical gauging with #25


centered in the canal; the smaller the ratio, the better the instrument remained centered in the canal<sup>9,18,19)</sup>

### 2-5. Questionnaires and Preference

Questionnaires with set questions were not used. Instead students gave their subjective opinions of each system's strong points, shortcomings, and specific difficulties. Each student indicated which system they preferred. Their preferences were analyzed.

### 3. Statistical analysis

Statistical analysis of the collected data was performed with SPSS™ version 10.0 (SPSS Inc., Chicago, IL, USA). The measured data was first checked for variance homogeneity by Levene's test. When the data had normal distribution, statistical analysis was performed with ANOVA and Scheffe test for post-hoc comparison. Differences revealed in the data were designated as significant at  $P < 0.05$ . When the data did not have a normal distribution, the nonparametric Kruskal-Wallis test and Bonferroni procedure were done.

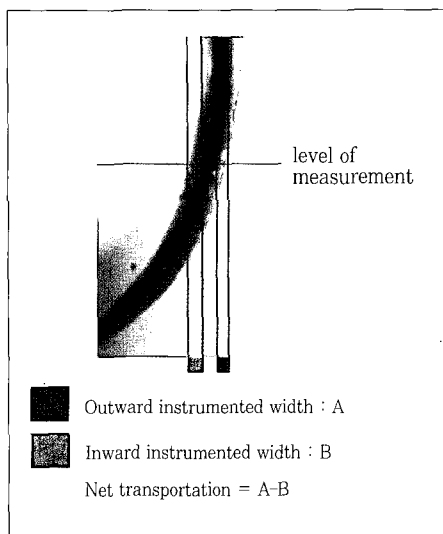

**Figure 1.** Instrumented canal width and net transportation.

## III . Results

### 1. Instrument distortion or breakage


There were only two broken files. One ProFile® .06 #25 and one rotary ProTaper® F1 were fractured by each student. The manual ProTaper® had no fractures and none of the three systems had other distortions or deformations.

### 2. Aberrations

The resin blocks instrumented with MPT or RPT had more zips and elbows than those with PF (Table 2).

### 3. Preparation time

The resin blocks that had procedural errors or other factors interfering with completion (such as instrument separation, ledge-not negotiated) were excluded from the samples for statistical analysis. The time needed for completion for each system is presented in Table 3. Students required more time for the entire preparation with the MPT system. The nonparametric Kruskal-Wallis test and

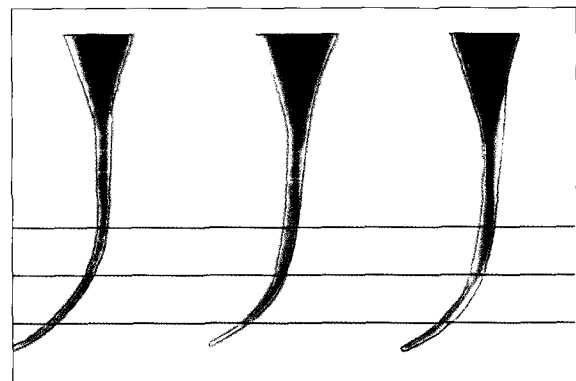

**Figure 2.** Three representative superimposed images after instrumentation by each Ni-Ti file systems: (Left) ProFile®, (Mid) manual ProTaper®, (Right) rotary ProTaper®. The three horizontal lines mean the measured levels of 1 mm, 3 mm, and 5 mm.

Bonferroni procedure showed statistically significant differences between the groups ( $P < 0.05$ ).

#### 4. Instrumented canal width, net transportation, and centering ratio

Three representative superimposed images of pre-instrumented and post-instrumented blocks are presented in Figure 2.

The instrumented canal widths in the RPT were significantly larger than those of the PF and MPT at the 1 mm and 3 mm levels. At the 5 mm level, both of the ProTaper® systems, MPT and RPT, enlarged the root canals more than PF ( $P < 0.05$ ) (Table 4).

There were no significant differences between the two ProTaper® groups in net transportation. However, the root canals prepared by the two ProTaper® systems deviated more than the ProFile® system at the 1 mm and 5 mm levels ( $P < 0.05$ ). Most of the deviations were inward with each of the ProTaper® systems having an outward deviations at the 1 mm level (Table 5).

The centering ratios at the 1 mm and 3 mm levels had no significant differences ( $P > 0.05$ ). The centering ratio at the 5 mm level was largest in MPT and the differences between the systems were significant ( $P < 0.05$ ) (Table 6).

**Table 2.** Incidence of canal aberrations by instrument types

	ProFile®	manual ProTaper®	rotary ProTaper®
Zip / Elbow	1	6	5
Ledge	1	2	2

**Table 3.** The lapse of time for each system (mean ± SD)

System	Sample	Preparation time
ProFile®	48	11 min 22 s ± 3 min 39 s
manual ProTaper®	48	20 min 20 s ± 7 min 1 s
rotary ProTaper®	48	8 min 8 s ± 2 min 33 s

**Table 4.** The instrumented canal width (mm) after root canal preparation (mean ± SD)

	ProFile®	manual ProTaper®	rotary ProTaper®
Level 5 mm	0.205 ± 0.065 <sup>a</sup>	0.392 ± 0.077 <sup>b</sup>	0.417 ± 0.070 <sup>b</sup>
Level 3 mm	0.174 ± 0.077 <sup>a</sup>	0.305 ± 0.079 <sup>b</sup>	0.346 ± 0.079 <sup>c</sup>
Level 1 mm	0.174 ± 0.075 <sup>a</sup>	0.364 ± 0.148 <sup>b</sup>	0.469 ± 0.109 <sup>c</sup>

<sup>abc</sup> Different letter indicates significant differences between the systems ( $P < 0.05$ ).

**Table 5.** The net transportations (mm) after root canal preparation (mean ± SD)

	ProFile®	manual ProTaper®	rotary ProTaper®
Level 5 mm	-0.139 ± 0.070 <sup>a</sup>	-0.336 ± 0.098 <sup>b</sup>	-0.301 ± 0.093 <sup>b</sup>
Level 3 mm	-0.082 ± 0.087	-0.093 ± 0.111	-0.122 ± 0.098
Level 1 mm	-0.078 ± 0.077 <sup>a</sup>	0.142 ± 0.154 <sup>b</sup>	0.139 ± 0.152 <sup>b</sup>

Negative value indicates an inward deviation.

<sup>abc</sup> Different letter indicates significant differences between the systems ( $P < 0.05$ ).

**Table 6.** The centering ratio (mean  $\pm$  SD)

	ProFile <sup>®</sup>	manual ProTaper <sup>®</sup>	rotary ProTaper <sup>®</sup>
Level 5 mm	0.304 $\pm$ 0.139 <sup>a</sup>	0.531 $\pm$ 0.122 <sup>b</sup>	0.441 $\pm$ 0.119 <sup>c</sup>
Level 3 mm	0.203 $\pm$ 0.148	0.198 $\pm$ 0.141	0.204 $\pm$ 0.128
Level 1 mm	0.192 $\pm$ 0.119	0.225 $\pm$ 0.161	0.207 $\pm$ 0.146

<sup>abc</sup> Different letter indicates significant differences between the systems ( $P < 0.05$ ).

**Table 7.** The summary of questionnaires

Item	ProFile <sup>®</sup>	manual ProTaper <sup>®</sup>	rotary ProTaper <sup>®</sup>
Preference	18	0	32
<b>Strong points :</b>			
Easy to handle	7	5	17
Feels safe	5	1	-
Efficient cutting	-	-	4
Preservation of tactile sense	-	9	-
<b>Shortcomings :</b>			
Time wasting	-	11	-
Difficult sequence	17	-	6
Aggressive cutting	-	-	12
Anxiety on instrument separation	-	-	9

- : no responses

## 5. Questionnaires and Preference

Students' responses are summarized in Table 7. While no students preferred MPT, however, 32 students preferred RPT over PF. Eleven students cited the length of time it took to operate the MPT as a disadvantage. Several students cited each system as being easy to handle (RPT 17, PF 7, and MPT 5). The safety about Ni-Ti file system was also mentioned. Five students indicated that they felt safe during the trial procedure using PF and one with MPT. However, RPT was not cited as feeling safe, nine students stated the anxiety about instrument breakage during use. In relation to tactile sense, nine students mentioned that MPT was more conservative than other systems. Twelve students complained that RPT often removed material aggressively and showed instru-

ment locking. In using ProTaper<sup>®</sup> systems (MPT and RPT), six students complained that F1 and F2 sequences were more difficult to follow and resistant than other steps. Similarly 17 students mentioned that the sequence from .04 #25 to .06 #20 in PF was difficult and resistant. Four students felt that the RPT's cutting ability was better and one student felt the same about MPT.

Finally, we evaluated and compared the simulated root canals instrumented by the two preferred groups. The 31 simulated canals prepared by RPT (a student's sample was excluded because of file fracture) and 18 canals by PF were evaluated. The data was analysed by Levene's test and *t*-test or nonparametric Mann-Whitney test. The statistical results were not different from that of previously described.

#### IV. Discussion

Rotary Ni-Ti instruments are used efficiently in root canal treatments throughout the world, but not by all dentists. It may not be common for most operators to practice on extracted teeth or plastic blocks to evaluate the possibilities and limitations of a new technique, device, or instrument<sup>11)</sup>. Like many clinical practitioners, most dental students do not have many opportunities to practice new techniques. The aim of this study was to evaluate the efficacy of the three Ni-Ti file systems used by undergraduates.

A survey about the use of rotary Ni-Ti instruments reported that these instruments were used by 22% of general dentists and 64% of endodontists<sup>20)</sup>. The two main reasons for not using rotary Ni-Ti were 'no perceived advantage' and 'high fragileness'. The next two most common problems encountered were 'binding' and 'ledging'. On the other hand, very high proportions of positive experiences were also noted.

The main problem inherent in rotary preparation by inexperienced operators is the risk of instrument fracture. A study<sup>9)</sup> that compare the breakage and distortion of various Ni-Ti file systems in curved canals reported that the ProFile<sup>®</sup> system had statistically significantly more distortions than the ProTaper<sup>®</sup> system. However, there was no distortion and little breakage in this study. The reason might be that the torque control motors were used for PF and RPT. The low-torque control motors will reverse the rotation of the instrument when the instrument is subjected to stress levels equal to the preset torque value<sup>21)</sup>. Most manufacturers suggest that the Ni-Ti instruments should be used about 10 times. The Ni-Ti files used in this study were new ones, so it is surmised that there were fewer fractures due to fatigue or over-use. Instrumentation technique, instrument design, angle and radius of canal curvature and the torque control motor all have an influence on the fracture rate of Ni-Ti files<sup>21-23)</sup>. Strictly, all of these factors do not always seem to exert an influence on beginners, dissimilarly on the experienced.

Statistical analysis of root canal aberrations was not possible due to the low number of occurrences. However, the MPT or RPT had a few more zips and elbows than the PF. The reason may be over-uses of F series files in ProTaper<sup>®</sup> system which can remove tooth structure excessively when left in the canal too long with their active design<sup>24)</sup>. It is therefore of utmost importance to follow the manufacturer's instructions and not to leave the RPT prepare the root canal for longer than 1 second or not to use the MPT too much when reaching the desired working length. These aberrations can be diminished with several pre-clinical trial uses and following the manufacture's instructions.

In the present study, the RPT took significantly less instrumentation time than the other systems. The same results were reported in other studies<sup>25,26)</sup> comparing the ProTaper<sup>®</sup> and other Ni-Ti rotary file systems. Statistically significant differences existed between the groups although there were large deviations in the amount of preparation time. It is natural that the manually controlled MPT would take longer to use. This was the reason that no student chose MPT as a preferred system. This statistically significant difference is, however, to be interpreted with caution, as the preparation times were recorded by students themselves and the time included not only actual instrumentation time but also the time for irrigation, changing instruments and recapitulation.

Manufacturers present the preservation of tactile sense as an advantage of the MPT system. However, beginners who had no experience using rotary file systems or even stainless steel files in clinical situations could not feel and did not need tactile sensation from the MPT. For this reason, they preferred the relatively fast and simple rotary systems.

Instrumented canal width simply implicates the cutting ability of the applied system. In this study, the canal width formed by MPT or RPT was significantly larger than that formed by PF. This seemed to be resulted from the thicker instrument, especially the F series files, which

have .07 (F1) or .08 (F2) apical taper in the ProTaper® system. Also, this might have resulted from the active cutting feature with that both ProTaper® systems have.

The studies<sup>27)</sup> that compared apical transportation between ProFile® and ProTaper® showed no statistically significant differences. However, in present study with the viewpoint of net transportations, all root canals usually deviated inwardly at all levels with exception of 1 mm level (the terminal point of the curvature) of MPT and RPT. At this level both ProTaper® systems had outward deviations. This tendency may have resulted from the greater restoring force of the ProTaper® file on the outer curve and the diminished super-elastic property of Ni-Ti due to the thick end of the ProTaper®, especially in F series files.

In centering ratio, there were significant differences at the only level of 5 mm between the systems and PF had the better centering ability than the other two groups at 5 mm level. Nevertheless, the centering ratios were not significantly different between the groups in level 1 mm and 3 mm. The results of the centering ratio can be used as an index for the capability of the instrument to stay centered in the canal. The centering ratio was used as one of the most important qualitative evaluations of the present study. In narrow and curved root canals, the coronal canals must be enlarged to facilitate access to the apical canal and obturation. The centering ratios at the 5 mm level indicate that both ProTaper® systems did not remain centered at the measured level of canal. Nevertheless, from the viewpoint of coronal flaring and obturation facilitation, the ProTaper® system can easily provide straight access to apically and larger apical sizes.

That no student preferred MPT was beyond expectation. Students' responses indicated that the RPT cut more canal wall more quickly than the PF did, which is in keeping with the previously cited material. This suggests that the shorter working time was seen as preferential by the students. The other advantages of the RPT the students cited were its ease of handling and effi-

ciency in cutting.

The constant tapered shaft design has more flexibility than the progressive tapered shaft design. And the U-shaped cross section is more flexible than the triangular cross section<sup>9,10)</sup>. The students seemed to react to the relatively rougher feel of the ProTaper® when compared to the ProFile®.

Properly used Ni-Ti file systems enable the user to finish more predictable root canal instrumentation and limit procedural errors at the same time<sup>10)</sup>. Generally, little information is available regarding the attitude of general dental practitioners towards new endodontic concepts, techniques and instruments, and on how far these have been incorporated into daily practice<sup>28)</sup>. Students have less bias towards the instruments and techniques, but quickly learn to manage the instrumentation system. The practitioners, however, who have biased information about the rotary Ni-Ti instrument initially began to use these instruments aggressively. This sometimes ended in breakage and failure of the instruments<sup>11)</sup>. So, it is suggesting that suitable preclinical training should be taken enough in advance of clinical practice on patients. It is advised to gain the requisite experience on 20 teeth including extracted teeth<sup>29)</sup>.

In this study, the ProFile® system represented a constant tapered and passive cutting file with negative rake angle and the recently introduced ProTaper® system as the only progressive tapered file on the market represented an active cutting file. The ProTaper® system is the only product that has two systems with different usage. Based on the results, novice operators even the students can do the root canal preparation with any of the Ni-Ti systems used in this study. Although the root canals instrumented using the ProTaper® systems showed a bit more cutting from a quantitative viewpoint, in the centering ratio of qualitative aspect, there were little differences between the three systems.

Based on the comparative report of mathematical models of ProTaper® and ProFile®, the results has shown that the ProTaper® model might be



more indicated for narrow canals and curved canals during the initial phase of shaping and that the ProFile® model might be more indicated for wider canals and curved canals in the final phase of shaping<sup>30</sup>. Further investigations such as hybrid techniques using various Ni-Ti file systems in the undergraduate students are needed prior to integrate the Ni-Ti file systems to regular undergraduate curriculum.

## V. Conclusions

Under the condition of this study, both ProTaper® systems allowed significantly more removal of root canal wall than the ProFile® system. In the important other aspects such as the centering ratio, there was no significant differences between the systems.

Senior dental students were able to prepare curved root canals with any Ni-Ti file systems with little aberration and great conservation of tooth structure. Students want to learn effective methods and at the same time simple rotary procedures. The rotary ProTaper® systems were one of the most compatible to these students from the point of view of cutting ability. The ProFile® system was also compatible in safe and gentle shaping.

## References

1. Deplazes P, Peters O, Barbakow F. Comparing apical preparations of root canals shaped by nickel-titanium rotary instruments and nickel-titanium hand instruments. *J Endod* 27(3):196-202, 2001.
2. Esposito PT, Cunningham CJ. A comparison of canal preparation with nickel-titanium and stainless steel instruments. *J Endod* 21(4):173-6, 1995.
3. Schafer E, Schulz-Bongert U, Tulus G. Comparison of hand stainless steel and nickel titanium rotary instrumentation: a clinical study. *J Endod* 30(6):432-5, 2004.
4. Coleman CL, Svec TA. Analysis of Ni-Ti versus stainless steel instrumentation in resin simulated canals. *J Endod* 23(4):232-235, 1997.
5. Garip Y, Gunday M. The use of computed tomography when comparing nickel-titanium and stainless steel files during preparation of simulated curved canals. *Int Endod J* 34(6):452-457, 2001.
6. Schafer E. Shaping ability of Hero 642 rotary nickel-titanium instruments and stainless steel hand K-Flexfiles in simulated curved root canals. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod* 92(2):215-220, 2001.
7. Hata G, Uemura M, Kato AS, Imura N, Novo NF, Toda T. A comparison of shaping ability using ProFile, GT file, and Flex-R endodontic instruments in simulated canals. *J Endod* 28(4):316-321, 2002.
8. Ankrum MT, Hartwell GR, Truitt JE. K3 Endo, ProTaper, and ProFile systems: breakage and distortion in severely curved roots of molars. *J Endod* 30(4):234-237, 2004.
9. Bergmans L, Van Cleynenbreugel J, Beullens M, Wevers M, Van Meerbeek B, Lambrechts P. Progressive versus constant tapered shaft design using NiTi rotary instruments. *Int Endod J* 36(4):288-295, 2003.
10. Clauder T, Baumann MA. ProTaper NT system. *Dent Clin North Am* 48(1):87-111, 2004.
11. Baumann MA, Roth A. Effect of experience on quality of canal preparation with rotary nickel-titanium files. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod* 88(6):714-718, 1999.
12. Gluskin AH, Brown DC, Buchanan LS. A reconstructed computerized tomographic comparison of Ni-Ti rotary GT files versus traditional instruments in canals shaped by novice operators. *Int Endod J* 34(6):476-484, 2001.
13. Sonntag D, Guntermann A, Kim SK, Stachniss V. Root canal shaping with manual stainless steel files and rotary Ni-Ti files performed by students. *Int Endod J* 36(4):246-255, 2003.
14. Sonntag D, Delschen S, Stachniss V. Root-canal shaping with manual and rotary Ni-Ti files performed by students. *Int Endod J* 36(11):715-723, 2003.
15. Hanni S, Schonenberger K, Peters OA, Barbakow F. Teaching an engine-driven preparation technique to undergraduates: initial observations. *Int Endod J* 36(7):476-82, 2003.
16. Qualtrough AJ, Dummer PM. Undergraduate endodontic teaching in the United Kingdom: an update. *Int Endod J* 30(4):234-239, 1997.
17. Qualtrough AJ, Whitworth JM, Dummer PM. Preclinical endodontology: an international comparison. *Int Endod J* 32(5):406-414, 1999.
18. Calhoun G, Montgomery S. The effects of four instrumentation techniques on root canal shape. *J Endod* 14(6):273-277, 1988.
19. Kosa DA, Marshall G, Baumgartner JC. An analysis of canal centering using mechanical instrumentation techniques. *J Endod* 25(6):441-445, 1999.
20. Parashos P, Messer HH. Questionnaire survey on the use of rotary nickel-titanium endodontic instruments by Australian dentists. *Int Endod J* 37(4):249-259, 2004.
21. Yared G, Bou Dagher F, Kulkarni K. Influence of torque control motors and the operator's proficiency on ProTaper failures. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod* 96(2):229-233, 2003.
22. Szep S, Gerhardt T, Leitzbach C, Luder W, Heidemann D. Preparation of severely curved simulated root canals using engine-driven rotary and conventional hand instruments. *Clin Oral Investig* 5(1):17-25, 2001.
23. Yared GM, Dagher FE, Machtou P, Kulkarni GK. Influence of rotational speed, torque and operator proficiency on failure of Greater Taper files. *Int Endod J* 35(1):7-12, 2002.
24. Calberson FL, Deroose CA, Hommez GM, De Moor RJ.

- Shaping ability of ProTaper nickel-titanium files in simulated resin root canals. *Int Endod J* 37(9):613-623, 2004.
25. Yun HH, Kim SK. A comparison of the shaping abilities of 4 nickel-titanium rotary instruments in simulated root canals. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod* 95(2):228-233, 2003.
  26. Schafer E, Vlassis M. Comparative investigation of two rotary nickel-titanium instruments: ProTaper versus RaCe. Part 1. Shaping ability in simulated curved canals. *Int Endod J* 37(4):229-238, 2004.
  27. Iqbal MK, Firic S, Tulcan J, Karabucak B, Kim S. Comparison of apical transportation between ProFile and ProTaper NiTi rotary instruments. *Int Endod J* 37(6):359-364, 2004.
  28. Slaus G, Bottenberg P. A survey of endodontic practice amongst Flemish dentists. *Int Endod J* 35(9):759-767, 2002.
  29. European Society of Endodontology. Undergraduate curriculum guidelines for endodontology. *Int Endod J* 34(8):574-580, 2001.
  30. Berutti E, Chiandussi G, Gaviglio I, Ibba A. Comparative analysis of torsional and bending stresses in two mathematical models of nickel-titanium rotary instruments: ProTaper versus ProFile. *J Endod* 29(1):15-9, 2003.

## 국문초록

# 학생들이 사용한 세 종류 Ni-Ti file systems의 근관성형 효율 비교

김현철 · 박정길 · 허 복\*

부산대학교 치과대학 치과보존학교실

이 연구의 목적은 Ni-Ti file을 사용한 경험이 없는 학생들이 세 종류 Ni-Ti file systems을 사용하였을 때 근관형성 효율을 비교하는 것이다.

Ni-Ti file의 사용 경험이 없는 부산대학교 치과대학 4학년 학생 50명이 세 종류의 Ni-Ti file systems - ProFile® (PF; Dentsply Maillefer, Ballaigues, Switzerland), manual ProTaper® (MPT; Dentsply Maillefer, Ballaigues, Switzerland), rotary ProTaper® (RPT; Dentsply Maillefer, Ballaigues, Switzerland) -을 사용하여 각 system으로 하나의 근관씩, 모두 150개의 레진 블록 근관모형(Endo Training Bloc; Dentsply Maillefer, Ballaigues, Switzerland)을 형성하였다. 근관형성에 사용된 file의 파절이나 변형 및 근관형성 후 형태의 이상을 조사하고, 스캐너로 근관 형성 전후의 이미지를 채득하여 중첩 비교함으로써 근단부로부터 1 mm, 3 mm, 그리고 5 mm 높이에서의 삭제된 근관의 폭경, 근관의 변위량, 그리고 중심변위를 등을 산출하고 통계학적 비교 분석을 하였다. 그리고 세 가지 systems에 관한 학생들의 주관적인 선호도를 조사하였다.

그 결과 졸업을 앞둔 치과대학 재학생들도 특별한 문제점 없이 세 가지 Ni-Ti file systems을 사용한 근관형성이 가능함을 확인하였다. 세 실험군을 비교하였을 때, 양적인 삭제 능력은 두 ProTaper® systems (manual and rotary)이 ProFile®에 비해 우수하였지만, 근관의 변위는 두 ProTaper® systems에서 더 많이 유발되었다. 근관 중심 이동률 등의 질적 평가를 포함하여 학생들의 선호도를 종합적으로 고려할 때, 삭제 능력에 있어서는 rotary ProTaper®가 더 효율적이지만 안전성을 고려하면 ProFile®도 추천된다. 정규 교육과정에 Ni-Ti file systems의 도입을 위해서 초심자와 관련한 더 많은 연구가 진행되어야 하겠다.

**주요어 :** 학생, 니켈-티타늄 파일, 성형 능력, 중심 변위를