

The Investigation of a Novel Indicator System for Trace Determination and Speciation of Selenium in Natural Water Samples by Kinetic Spectrophotometric Detection

Ramazan GÜRKAN* and Halil İbrahim ULUSOY

University of Cumhuriyet, Faculty of Science & Arts, Department of Chemistry, TR-58140, Sivas, Turkey

*E-mail: rgurkan@cumburiyet.edu.tr

Received February 11, 2010, Accepted May 6, 2010

A novel catalytic kinetic method is proposed for the determination of Se(IV), Se(VI) and total inorganic selenium in water based on the catalytic effect of Se(IV) on the reduction of bromate by *p*-nitrophenylhydrazine at pH 3.0. The generated bromine, Br₂ or Cl₂ plus Br₂ in 0.1 M NaCl (or NaBr) environment efficiently decolorized Calmagite and the reaction was monitored spectrophotometrically at 523 nm as a function of time. In this indicator reaction, bromide acted as an activator for the catalysis of selenium (IV) and a reducing agent for selenium (VI) at pH 3.0, which allowed the determination of total selenium. The fixed time method was adopted for the determination and speciation of inorganic selenium. Under the optimum conditions, the calibration graph are linear in the range 1 - 35 µg L⁻¹ of Se(IV) for the fixed time method at 25 °C. The detection limit based on statistical 3S_{blank}/m-criterion was 0.215 µg L⁻¹ for the fixed time method (7 min). All of the variables that affect the sensitivity at 523 nm were investigated, and the optimum conditions were established. The interference effect of various cations and anions on the Se (IV) determination was also studied. The selectivity of the selenium determination was greatly improved with the use of the strongly cation exchange resin such as Amberlite IR120 plus. The proposed kinetic method was validated statistically and through recovery studies in natural water samples. The RSDs for ten replicate measurements of 5, 15 and 25 µg L⁻¹ of Se(IV) and Se(VI) was changed between 2.1 - 4.85%. Analyses of a certified standard reference material (NIST SRM 1643e) for selenium using the fixed-time method showed that the proposed kinetic method has good accuracy. Se(IV), Se(VI) and total inorganic selenium in environmental water samples have been successfully determined by this method after selective reduction of Se(VI) to Se(IV).

Key Words: Selenium speciation and determination, Calmagite, Catalytic effect, Kinetic spectrophotometry, Natural waters

Introduction

The determination of selenium in natural waters has received great attention during the past years owing to the biological importance of this element. Selenium is an essential trace element but at elevated levels it is toxic to biological systems.¹⁻² It is generally recognized that the toxicity and the bioavailability are controlled not only by the total concentration but also by the chemical forms. The physiological behavior of selenium is dependent upon its oxidation state Se(IV), Se(VI) and Se(-II), selenide being generally present in organic forms (selenocysteine, selenomethionine, methylated compounds). The concentration of selenium generally encountered in natural waters is in the ng L⁻¹ or sub-mg L⁻¹ range. So it is important to have selective and sensitive methods to identify each species and determine their levels.

Over the past two decades various instrumental techniques including UV-visible spectrophotometry,³ atomic/molecular fluorescence spectrometry,⁴⁻⁷ high performance liquid chromatography,⁵ hydride generation atomic absorption spectrometry,⁸⁻¹² differential pulse cathodic stripping voltammetry,¹³ inductively coupled plasma mass spectrometry,¹⁴ ion chromatography¹⁵⁻¹⁶ and flow injection analysis coupled with hydride generation atomic fluorescence spectrometry¹⁷ have been developed and used for Se speciation.

However, the catalytic kinetic spectrophotometric methods offer distinct advantages for being of high sensitivity, low cost

and simplicity for a large majority of analytes in water samples.¹⁸⁻²² A significant number of methods for selenium determination in real samples are based on catalytic effect of Se(IV) on the reduction of dyes such as Toluidine blue,²³ Methylene blue,²⁴ Gallocyanin,²⁵ Semicarbazide²⁶ and Ponceau S.²⁷ Some of these methods have high limit of detection, or suffer from many interfering ions such as Te(IV) and As(III), or have time consuming procedures, or these reagents used are unstable. Additionally, few catalytic kinetic methods for the determination of Se(IV) in water systems have been reported in the literature as presented in Table 1²⁸⁻³⁵ but only one catalytic kinetic method³⁶ exists which allows the determination of Se(IV), Se(VI) and total inorganic Se in water samples. Therefore, there is still need to develop the more sensitive and selective catalytic kinetic spectrophotometric method for the determination and speciation of selenium in real samples.

We found that bromate slowly reacts with *p*-nitrophenylhydrazine using Calmagite as chromogenic reagent in weak acidic media and Se(IV) catalytically accelerates this reduction reaction at 523 nm. In the present study, a sensitive and selective catalytic spectrophotometric method is described for the determination of Se(IV) and Se(VI) by using reduction of Se(VI) to Se(IV) and the Se(IV)-catalyzed reaction of bromate with *p*-nitrophenylhydrazine in the presence of Calmagite. The proposed method could simultaneously determine Se(IV) and (IV + VI) in the concentration range of 1 - 35 µg L⁻¹ without serious interferences, which allows to monitor easily the selenium species.

Table 1. Comparison of some catalytic kinetic spectrophotometric methods for determination of selenium in natural waters and real samples

Reagents	Detection limit, detection range, $\mu\text{g L}^{-1}$ or $\mu\text{g mL}^{-1}$	Remarks	Sample(s)	Ref.
Toluidine blue, Sulfide	0.08, 0.2 - 2	Flow injection spectrophotometry, The method is suitable for routine analysis; about 35 samples can be injected per hour.	Ores and pharmaceutical preparations	[23]
Methylene blue, Sulfide	2.5 - 30	Induction period method, the catalytic method was applied to urine samples with 84.9% recovery	Blood, hair and urine samples	[24]
Gallocyanin, Sulfide	0.002, 0.010 - 0.500	620 nm, 30 °C	Real samples	[25]
Semicarbazide, Hydrazine, Bromate	43, 50 - 4000	The method is based on the catalytic effect of Se(IV) in redox reaction of bromate with semicarbazide in hydrochloric acid media.	Kjeldahl tablets and a health-care product	[26]
Ponceau S, Bromate, Hydrazine	3.3, 4.5 - 400	525 nm, initial rate(or slope) method, pH 1.4, 40 °C, There is a serious interfering arising from As(III) and Te(IV) ions	Spiked water, kjeldahl tablet, Selenium tablet, Shampoo	[27]
Bromate, Hydrazine sulfate, Ascorbic acid, Activated carbon, Methyl orange	0.012, 0.02 - 20.0	525 nm, preconcentration of Se, fixed time method (30s), recovery 89 - 105%, RSD 1.0 - 7.1% for Se(IV) and Se(VI)	Environmental water	[28]
Methylene blue, Sulfide	2.5 - 30	668 nm, interference removed with organic solvents, room temperature; recovery 91.8% and RSD 2.3% for 15 ppb	Natural water	[29]
Maxilon blue-SG, Sulfide	0.205, 0.004 - 0.200	654 nm, fixed time method (4.0 min), 30.0 °C, pH 6.5, interference removed by cation-exchange resin, recovery > 91%, RSD < 2.27% for 0.004 - 0.16 $\mu\text{g mL}^{-1}$	Spring water	[30]
Sulfonazo, Sulfide	0.3, 0.5 - 180 and 50 - 2300	680 nm, by fixed time method; interference removal with cation exchange resin	Natural and synthetic water	[31]
<i>p</i> -Hydrazinobenzene-sulfonic acid (HBS), <i>N</i> -(1-Naphthyl) ethylene-diamine (NED), Bromide	0.2 - 6	538 nm, flow injection with two schemes, 25 °C and 100 °C, RSD 1.2 and 1.3% for 3 ng mL ⁻¹ Se(IV) and Se(VI) (<i>n</i> = 10)	Natural water	[32]
Iron(II) ethylenediamine-tetraacetate, 4-Nitroaniline, Nitrate, <i>N</i> -Diethyl- <i>N</i> -(1-naphthyl)-ethylenediamine	0.1	540 nm, interference removal by ultrasonic treatment, RSD 6% and 2% for 0.2 and 2 ng mL ⁻¹ Se	Potable and natural water	[33]
Ethylenediamine tetracetic acid disodium salt (EDTA), Nitrate, Ammonium iron(II) sulfate hexahydrate	2.5 - 200 and 200 - 2000	Flow injection with 7 samples h ⁻¹ , recovery 95 - 104%, RSD 3.4% for 5 × 10 ⁻⁸ g mL ⁻¹ Se(IV) (<i>n</i> = 11), 2.7% for 5 × 10 ⁻⁷ g mL ⁻¹ Se(IV) (<i>n</i> = 11)	Seawater	[34]
4,5-Dihydroxy-3-(<i>p</i> -sulfo-phenylazo)-2,7-naphthalene disulfonic acid, Sulfide	0.3, 0.5 - 100	515 nm, RSD 2.10 and 1.95% for 0.02 and 0.10 $\mu\text{g mL}^{-1}$ Se(IV), fixed time method (2.5 - 7.0 min)	Natural water	[35]
Bromate, Hydrazine dihydrochloride, Methyl orange	1.3, 0 - 789.6	507 nm, recovery 97 - 102%, RSD < 6% for 31.6 - 126.3 $\mu\text{g L}^{-1}$ Se(IV) and Se(VI) (<i>n</i> = 5), 25 °C, pH 1.6, fixed time (5 min) and initial rate methods	Drinking, natural and synthetic water	[36]
Bromate, <i>p</i> -Nitrophenyl-hydrazine, Calmagite	0.215, 1 - 35	523 nm, recovery 99.2 - 105%, RSD 2.1 - 4.85% for 2 - 20 $\mu\text{g L}^{-1}$ of Se(IV) and Se(VI) (<i>n</i> = 5), 25 °C, pH 3.0 acetate buffer, fixed time (7 min) method	River water, lake water and certified Standard reference material	The present study

The method has successfully been applied to the determination of Se(IV) and (VI) in spiked natural water samples such as lake water and river water.

Experimental

Apparatus. In the present study, a Shimadzu model UV-visible 1601 PC spectrophotometer equipped with a 1 cm quartz cell and a temperature-controlled cell holder (TCC-140A) was used for absorbance measurements at a fixed wavelength of 523 nm. A Grant LTG-6G model thermostatic water bath was used to control the temperature of reaction medium with an accuracy of ± 0.1 °C. A stopwatch was used for recording the reaction time. All solutions were preheated to a temperature of 25 °C shortly before the initiation of indicator reaction with and without catalyst. A Sartorius Docu-model pH meter supplied with a combined electrode pH meter was calibrated with standard buffers of pH 4.0 ± 0.1 and 7.0 ± 0.1 and used for measuring pH of solutions.

Reagents and solutions. All chemicals were of analytical reagent grade. All solutions were made up in Triply distilled, de-ionized water. A 0.01 M Se(IV) standard solution was prepared by dissolving 0.173 g of Na_2SeO_3 in 100 mL water. A 0.01 M Se(VI) standard solution was prepared by dissolving 0.1889 g of Na_2SeO_4 in 100 mL water. A 1000 mg L^{-1} stock calmagite solution was prepared by dissolving 0.10 g of calmagite in 100 mL water. A 0.05 M bromate solution was prepared by dissolving 0.835 g KBrO_3 in 100 mL water. A 0.05 M *p*-nitrophenylhydrazine solution was prepared by dissolving 0.5249 g *p*-nitrophenylhydrazine in approximately 2 mL 2 M H_3PO_4 and diluting with water up to 100 mL water. The HAc/Ac buffer solution of 100 mL pH 3 was prepared from 0.1 M HAc and 1.0 M NaAc solutions.

General procedure. All solutions were thermally equilibrated at 25 °C in a thermostatic water bath before addition of reagents. A suitable portion of Se(IV) solution in the range of 1 - 35 $\mu\text{g L}^{-1}$ was added into a 10 mL calibrated flask, then 1.5 mL of pH 3.0

HAc/Ac buffer solution, 0.5 mL 0.005 M *p*-nitrophenylhydrazine and 0.7 mL 0.05 M BrO_3^- were added and the solution was diluted to about 7 mL. After 2.5 mL 50 mg L^{-1} calmagite was added, the mixture was diluted to 10 mL. Time was measured just after the addition of the last drop of calmagite solution. The solution was mixed and a portion of that was transferred within 30 s into a 1 cm spectrophotometric cell to measure the absorbance change (ΔA_C) against water at 523 nm over the period 0.5 - 7.0 min after the initiation of the reaction by using fixed-time method. By the use of a serial of standard Se(IV) solution, a calibration graph of net change of absorbance, $\Delta(\Delta A)$ at a fixed time *versus* selenium (Se(IV)) concentration was constructed. The detailed calibration data are given in Table 2 as follows.

Recommended procedures for inorganic Se speciation in water samples. Selenium content in water samples was found below the detection limit of the method. Thus the environmental water samples were spiked simultaneously with Se(IV) and Se(VI) standards giving three different concentrations of 5, 10 and 20 $\mu\text{g L}^{-1}$ and the recovery for Se(IV) was carried out using fixed time method of 7 min. The content of Se(VI) in the spiked samples was determined after reducing procedures.³⁷ For reduction 25 mL of the spiked solution was mixed with 25 mL of 12 M HCl in a 100 mL capped hard glass test-tube and heated in a water bath at 90 °C for 30 min where Se(VI) is quantitatively reduced to Se(IV). The resulting solution was diluted to 100 mL with 6 M NaOH solution to adjust the pH.³⁷ The analysis for total Se(IV) was carried out using recommended fixed time method. The Se(VI) was determined as a difference between the recovered total inorganic Se(IV) found after reduction and Se(IV) found without reduction.

Results and Discussion

Preliminary studies. For the optimization of indicator reaction, the impact of reaction variables such as KBrO_3 , *p*-nitrophenylhydrazine, calmagite, ionic strength and temperature

Table 2. Analytical characteristics for the determination of [Se(IV)] using fixed time method in the range 1 - 35 $\mu\text{g L}^{-1}$ under optimum conditions of [Calmagite] = 12.5 mg L^{-1} , $[\text{BrO}_3^-] = 3.5 \times 10^{-3}$ M, [*p*-nitrophenylhydrazine] = 2.5 $\times 10^{-3}$ M, 1.5 mL pH 3 acetate buffer, temperature = 25 °C at λ_{max} : 523 nm

Parameters	Fixed-time method					
	1 min	3 min	5 min	7 min	9 min	12 min
Linear dynamic range, ng mL^{-1}	1 - 35	1 - 35	1 - 35	1 - 35	1 - 35	1 - 35
Linear regression equation	$\Delta A_1 = 9.96 \times 10^{-5}$ [Se(IV), ng mL^{-1}] $- 1.19 \times 10^{-4}$	$\Delta A_3 = 2.25 \times 10^{-4}$ [Se(IV), ng mL^{-1}] $- 1.87 \times 10^{-4}$	$\Delta A_5 = 3.46 \times 10^{-4}$ [Se(IV), ng mL^{-1}] $- 8.86 \times 10^{-4}$	$\Delta A_7 = 3.95 \times 10^{-4}$ [Se(IV), ng mL^{-1}] $- 2.40 \times 10^{-3}$	$\Delta A_9 = 4.64 \times 10^{-4}$ [Se(IV), ng mL^{-1}] $- 2.55 \times 10^{-3}$	$\Delta A_{12} = 4.87 \times 10^{-4}$ [Se(IV), ng mL^{-1}] $- 2.86 \times 10^{-3}$
Correlation coefficient (r)	0.9942	0.9955	0.9975	0.9985	0.9768	0.9634
^a Detection limit, ng mL^{-1}	13.75	5.62	2.76	0.215	1.85	4.54

^aBased on statistical $3S_{\text{blank}}/m$ -criterion for ten replicate blank absorbance change (ΔA_0) measurements



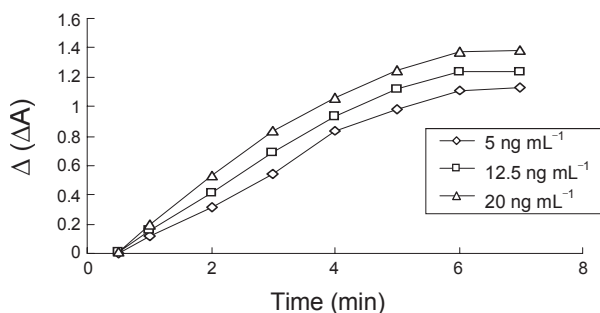


Figure 1. Effect of time on analytical sensitivity for the net reaction rates in the presence of 5, 12.5 and 20 $\mu\text{g Se(IV) L}^{-1}$. Optimum conditions: [Calmagite] = 12.5 mg L^{-1} , $[\text{BrO}_3^-] = 3.5 \times 10^{-3} \text{ M}$, [*p*-nitrophenylhydrazine] = $2.5 \times 10^{-3} \text{ M}$, temperature = 25 $^\circ\text{C}$, fixed-time, 7 min at 523 nm.



of environment on analytical sensitivity, $\Delta(\Delta A)$ was investigated. It was found that the maximum change in absorbance as analytical signal ($\Delta(\Delta A)$: $\Delta A_C - \Delta A_0$) was occurred within the first 7 min passing after the initiation of the catalytic reaction. Under optimum conditions, it was found that there is a linear relationship with an increasing slope for the selenium concentrations of 5, 12.5 and 20 $\mu\text{g L}^{-1}$ between analytical signal and reaction time for the first 7 min. For this reason, the fixed-time measurement of 7-min was chosen as the most suitable reaction time for the determination of selenium in real samples (Figure 1).




The catalytic reaction mechanism. Calmagite, with the chemical name of 2-hydroxy-1-(2-hydroxy-5-methylphenylazo)-4-naphthalenesulfonic acid, is an azo dye, which is used as indicator for Ca^{2+} and Mg^{2+} ions in water hardness measurement and also used as a redox indicator. The decolorization of Calmagite in presence of bromate ion is quite slow in weak acidic media. However, Se(IV) catalytically accelerates this reaction in weak acidic media but the catalysis is too fast to be monitored spectrophotometrically. The addition of *p*-nitrophenylhydrazine in the reaction medium slows down the reaction rate. A reasonable catalytic route of Se is that the *p*-nitrophenylhydrazine reduce Se(IV) or SeOBr_2 to elemental Se quantitatively in acidic medium as shown in Eq. (4). The elemental Se thus formed is oxidized back to Se(IV) by BrO_3^- , generating Br^- {Eq. (5)}. The Br^- in acidic medium is oxidized by BrO_3^- to Br_2 {Eq. (6-7)} which oxidizes i.e. decolorizes Calmagite as shown in Eq. (5) and similar observations have been obtained by other workers. Thus, the oxidation of Calmagite is significantly accelerated in presence of trace quantities of Br_2 i.e. indirectly it is catalyzed in the presence of trace quantities of Se(IV) {Eq. (8)}. An evident increase, which is observed in rate of Se(IV)-catalyzed reaction at 523 nm may be attributed to a formation of SeOBr_2 as a reactive intermediate, formed in the activation step of indicator reaction with bromide as follows:





Again, dependence of catalyzed-reaction rate on acidity and activator concentration in determination of total selenium can be attributed to a nucleophilic attack of the bromide ion on protonated form of selenic acid in prereduction of Se(VI) to Se(IV) in acid medium in the temperature range of 20 - 35 $^\circ\text{C}$.





This intermediate product, HSeO_3Br then undergoes further reactions, following the overall process:



This interpretation based on consideration as a nucleophile rather than a reducing agent is also supported by the smaller reactivity of chloride ions as can be seen in Figure 8. As the formation of Se(IV) is controlled by reaction (2) as the rate determining step, rate of reactions summarized in Eq. (3) must be faster than the rate of the sequence (1) and (2). As reaction (3) is faster than reaction (2), no direct evidence is available about the sequence of steps in process (3). Nonlinear dependence of sensitivity as analytical signal on concentration of bromide ions may be due to participation of bromide ions in step (3). It could be concluded that the above observations and conclusions in this context will be useful in a development of a more reliable procedure for determination of Se(VI) in mixtures with Se(IV) in real samples.



In the presence of 0.15 M NaCl or NaCl plus NaBr,

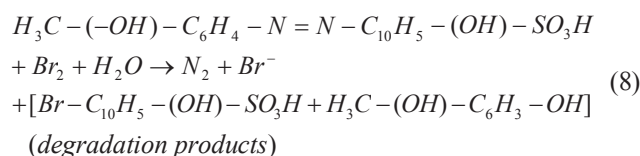

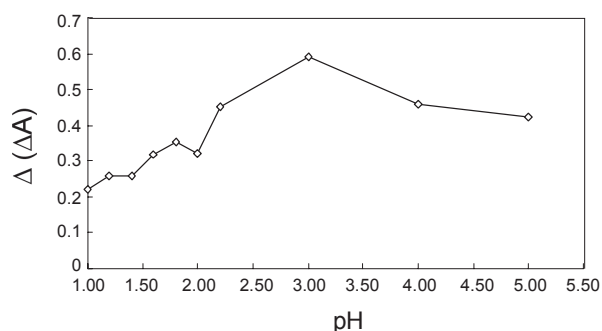


Figure 2. Effect of pH on analytical sensitivity for the net reaction rates. Optimum conditions: [Calmagite] = 12.5 mg L⁻¹, [BrO₃⁻] = 3.5 × 10⁻³ M, [*p*-nitrophenylhydrazine] = 2.5 × 10⁻³ M, temperature = 25 °C, fixed-time, 7 min at 523 nm.

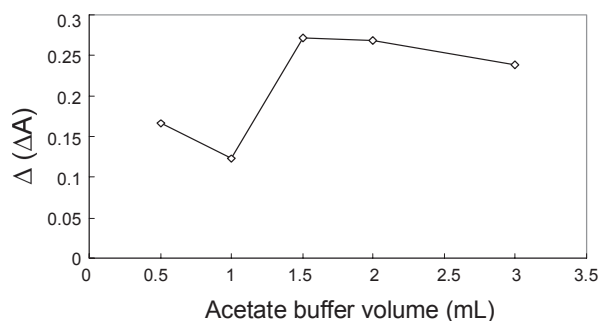


Figure 3. Effect of buffer volume on analytical sensitivity for the net reaction rates. Optimum conditions: [Calmagite] = 12.5 mg L⁻¹, [BrO₃⁻] = 3.5 × 10⁻³ M, [*p*-nitrophenylhydrazine] = 2.5 × 10⁻³ M, pH 3.0 acetate buffer, temperature = 25 °C, fixed-time, 7 min at 523 nm.

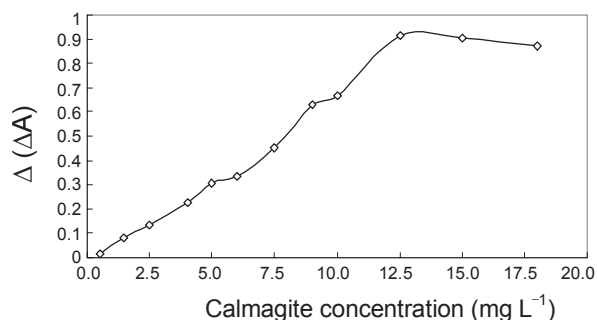


Figure 4. Effect of Calmagite concentration on analytical sensitivity for the net reaction rates. Optimum conditions: [BrO₃⁻] = 3.5 × 10⁻³ M, [*p*-nitrophenylhydrazine] = 2.5 × 10⁻³ M, 1.5 mL pH 3.0 acetate buffer, temperature = 25 °C, fixed-time, 7 min at 523 nm.

It is well known³⁸⁻⁴² that most indicator reactions used for kinetic-catalytic determination of selenium at trace amounts (where Methyl orange as chromogenic reagent is used) are based on oxidation-reduction reactions in which the catalyst that is usually a multi-charged ion such as Se(IV) and/or Se(VI) changes its oxidation state during the reaction especially in the presence of reducing agents such as hydrazine, hydroxyl amine and ascorbic acid. Therefore, the possible catalytic reaction mechanism for the indicator system in pH 3.0 acetate buffer media may be suggested by a series of reactions as the above-

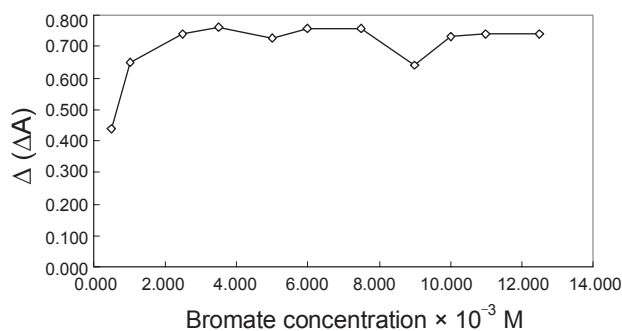


Figure 5. Effect of bromate concentration on analytical sensitivity for the net reaction rates. Optimum conditions: [Calmagite] = 12.5 mg L⁻¹, [*p*-nitrophenylhydrazine] = 2.5 × 10⁻³ M, 1.5 mL pH 3.0 acetate buffer, temperature = 25 °C, fixed-time, 7 min at 523 nm.

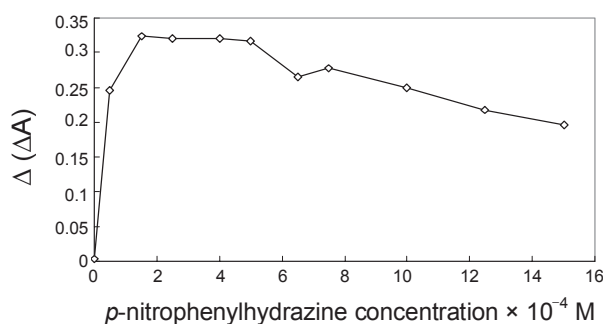


Figure 6. Effect of *p*-nitrophenylhydrazine concentration on analytical sensitivity for the net reaction rates. Optimum conditions: [Calmagite] = 12.5 mg L⁻¹, [BrO₃⁻] = 3.5 × 10⁻³ M, 1.5 mL pH 3.0 acetate buffer, temperature = 25 °C, fixed-time, 7 min at 523 nm.

mentioned.

The optimization of analytical variables. The effect of pH on the rate of the net catalyzed reaction was studied in the pH range 1.0 - 5.0 as shown in Figure 2. It can clearly be seen that the maximum sensitivity obtained near to 3.0. Therefore, pH 3.0 was chosen as optimum for further studies. In order to remain constant the pH of indicator system the effect of the buffer concentration was also examined. The results indicated that 1.5 mL was optimum amount of NaAc-HAc buffer (Figure 3).

The effect of calmagite concentration on reaction rates was studied for a concentration range of 0 - 20 mg L⁻¹. The present study has shown that both the catalyzed and uncatalyzed reaction rates increase with increase in calmagite concentration up to 12.5 mg L⁻¹ (Figure 4). For convenience and reliability, a calmagite concentration of 12.5 mg L⁻¹ was chosen as optimum value for further studies.

The effect of the concentration of BrO₃⁻ on the net reaction rate was studied in its concentration range 5 × 10⁻⁴ to 1.3 × 10⁻² M. Increasing concentration of BrO₃⁻ increases rates for both the uncatalyzed and catalyzed reactions in the range of 5 × 10⁻⁴ to 7.5 × 10⁻³ M. At the concentration range studied, the net reaction rate continued to increase with increasing concentration of BrO₃⁻ (Figure 5). Hence, a concentration of 3.5 × 10⁻³ M was chosen for further studies.

The effect of the concentration of *p*-nitrophenylhydrazine was studied for the concentration range of 0 - 15 × 10⁻⁴ M. The

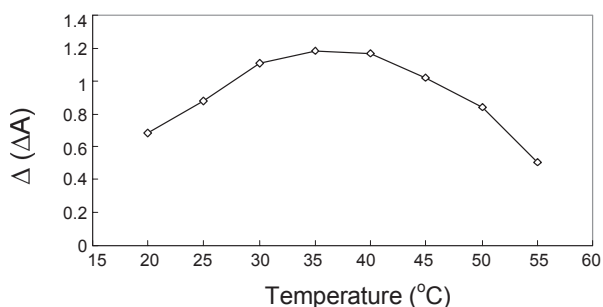


Figure 7. Effect of temperature on analytical sensitivity for the net reaction rates. Optimum conditions: [Calmagite] = 12.5 mg L⁻¹, [*p*-nitrophenylhydrazine] = 2.5 × 10⁻³ M, [BrO₃⁻] = 3.5 × 10⁻³ M, 1.5 mL pH 3.0 acetate buffer, fixed-time, 7 min at 523 nm.

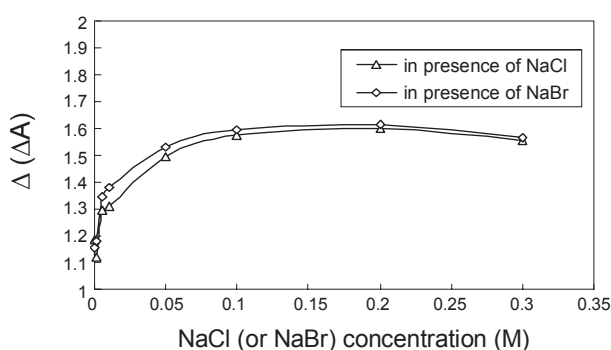


Figure 8. Effect of ionic strength on analytical sensitivity for the net reaction rates. Optimum conditions: [Calmagite] = 12.5 mg L⁻¹, [*p*-nitrophenylhydrazine] = 2.5 × 10⁻³ M, [BrO₃⁻] = 3.5 × 10⁻³ M, 1.5 mL pH 3.0 acetate buffer, temperature = 25 °C, fixed-time, 7 min at 523 nm.

plot of initial rate against the concentration of *p*-nitrophenylhydrazine is shown in Figure 6. It clearly indicates that the uncatalyzed and catalyzed reactions rates increase with increasing concentration of *p*-nitrophenylhydrazine until 2.5 × 10⁻⁴ M, where the net reaction rate starts leveling off between the range of (1.75 - 5.5) × 10⁻⁴ M (Figure 5). Therefore, 2.5 × 10⁻⁴ M was chosen as the optimum concentration of *p*-nitrophenylhydrazine.

Under the optimum conditions the effects of reaction temperature on the net reaction rate was investigated in the range of 20 - 55 °C. It was observed that increasing temperature of the catalyzed and uncatalyzed reactions accompanied an increase in the rates of reaction. The temperature of 25 °C gives stable catalyzed reaction rates while the uncatalyzed reaction rate was relatively low and stable. Therefore, 25 °C was the chosen temperature for all subsequent study and analyses (Figure 7).

The ionic strength dependence on the catalyzed and uncatalyzed reaction was studied in the range of 0 - 0.30 M (NaCl or NaBr). A plot of ionic strength in terms of the concentration of NaCl or NaBr *versus* the net reaction rate showed that the catalytic reaction rates dramatically increased with increasing ionic strength up to 0.10 M for both salt solutions. However, the analytical sensitivity in the presence of NaBr increased with a larger slope than those of NaCl in the range of 0 - 0.1 M. Therefore, a concentration of approximately 0.15 M was considered as optimum value for further study (Figure 8).

Table 3. Effect of interfering ions on the determination of 12.5 μg L⁻¹ Se(IV) under optimum conditions ([Calmagite] = 12.5 mg L⁻¹, [*p*-nitrophenylhydrazine] = 2.5 × 10⁻³ M, 1.5 mL pH 3.0 acetate buffer, temperature = 25 °C, fixed-time, 7 min at 523 nm) and using the regression equation based on fixed time method given in Table 2

Interfering ion	Tolerance limit, C _{interfering ion} /C _{Se(IV)}
K ⁺ , Na ⁺ , Li ⁺ , NH ₄ ⁺ , Ca ²⁺ and Mg ²⁺	5000 ^a
Cl ⁻ , F ⁻ , CO ₃ ²⁻ , HCO ₃ ⁻ , H ₂ PO ₄ ⁻ , Mn ²⁺ , C ₂ O ₄ ²⁻ , CH ₃ COO ⁻ and ClO ₃ ⁻	1000
NO ₃ ⁻ , Fe ²⁺ , Al ³⁺ , Cr ³⁺ , Zn ²⁺ and Ni ²⁺	500
V ⁴⁺ , Ce ³⁺ and CrO ₄ ²⁻	250
I ₂ , C ₂ O ₄ ²⁻ , Sn ²⁺ and SeO ₄ ²⁻	100
Pb ²⁺ , Co ²⁺ , MoO ₄ ²⁻ , SO ₃ ²⁻ , I ⁻	75
Cu ²⁺ , IO ₃ ⁻ , NO ₂ ⁻ , Br ⁻ , SCN ⁻	50
V ⁵⁺ , Ce ⁴⁺ , As ³⁺ , Sb ³⁺ and Fe ³⁺	15
Hg ²⁺	1
Sn ²⁺ , Pb ²⁺ , Co ²⁺ , Cu ²⁺ , V ⁵⁺ , Ce ⁴⁺ , Fe ³⁺ , As ³⁺ and Sb ³⁺	750 - 1250 ^b

^aMaximum tolerance limit tested. ^bAfter using the cation-exchange resin.

Table 4. The accuracy and precision of the proposed kinetic method for the determination of Se(IV) and Se(VI) under the optimum conditions ([Calmagite] = 12.5 mg L⁻¹, [*p*-nitrophenylhydrazine] = 2.5 × 10⁻³ M, 1.5 mL pH 3.0 acetate buffer, temperature = 25 °C, fixed-time, 7 min at 523 nm)

Added (ng mL ⁻¹)	Found (ng mL ⁻¹)	Precision (ng mL ⁻¹) ^a	Accuracy, %Relative Error ^b
2.0	-	2.10	C = 2.10 ± 0.05 S _C = 0.10 RSD = 4.76%
10.0	-	9.92	C = 9.92 ± 0.07 S _C = 0.14 RSD = 1.41%
20.0	-	19.88	C = 19.88 ± 0.02 S _C = 0.05 RSD = 0.25%
3.0	3.05	3.05	C = 3.05 ± 0.02 S _C = 0.04 RSD = 1.31%
6.0	5.96	5.96	C = 5.96 ± 0.02 S _C = 0.04 RSD = 0.67%
12.0	12.12	12.12	C = 12.12 ± 0.03 S _C = 0.07 RSD = 0.58%

^aThe mean plus its standard error (C), standard deviation (S_C) and relative standard deviation (RSD) for five replicate measurements.

^bAccuracy = [(Found-Added)/Added] × 100.

Analytical data.

Analysis by the fixed-time method: Calibration graph of change in absorbance at a fixed time (Δ(ΔA)_t) *versus* concentration of Se(IV) at eight different concentrations were plotted at a fixed time (t = 1, 3, 5, 7, 9 and 12 min) in the range 1 - 35 μg L⁻¹.

Table 5. Determination of Se(IV) and Se(VI) in natural river water^a and lake water^b samples

Sample	Se(IV), ng mL ⁻¹		Se(VI), ng mL ⁻¹	
	Added	Found ^c	Added	Found ^c
River water (Kızılırmak, Sivas)	-	1.39 ± 0.03	-	2.68 ± 0.03
	5.0	6.43 ± 0.03	-	-
	10.0	11.36 ± 0.02	-	-
	20.0	21.42 ± 0.02	-	-
	-	-	5.0	4.92 ± 0.03
	-	-	10.0	9.96 ± 0.02
	-	-	20.0	19.94 ± 0.02
Lake water (Hafik, Sivas)	-	< 0.2	-	< 0.2
	5.0	5.04 ± 0.02	-	-
	10.0	9.97 ± 0.03	-	-
	20.0	19.95 ± 0.03	-	-
	-	-	5.0	4.98 ± 0.04
	-	-	10.0	10.3 ± 0.03
	-	-	20.0	20.05 ± 0.02

^aThe river water samples were collected from Kızılırmak River, Sivas in Turkey on June 2009. ^bThe lake water samples were collected from Hafik Lake, Sivas in Turkey on June 2009. ^cAverage of six replicate determinations ± S.D.

It is apparent from Table 2 that the values of error, RSDs and detection limits were found to be lowest for fixed time of 7 min for 1 - 35 µg L⁻¹ Se(IV), respectively. Therefore, the fixed time of 7 min was adopted with the highest sensitivity and correlation coefficient for the analysis of inorganic Se in water samples.

Selectivity of indicator reaction: In order to establish the application of the proposed method to environmental samples, the selectivity of the proposed method was evaluated by determining 15 µg L⁻¹ of Se(IV) in the presence of varying amounts of cations and anions which are commonly present in environmental waters. The tolerance limit was defined as the concentration of an added ion causing not more than ± 3% relative error⁴³ and the results are summarized in Table 3. The interference effect of cations could be removed by passing the solution through a column containing a strongly cation-exchange resin. The tolerance limit was increased up to a value changing the range of 750 - 1250 for each interfering species with Amberlite IR120 plus as a cation-exchange resin. It was found that many of these ions did not interfere, even when present in excess of 5000 to 50 fold. Those ions which interfere, if present greater than 10 fold excess, are seldom present at the concentrations levels tested in natural waters.⁴⁴ Thus the proposed method is suitable for the determination of inorganic Se in environmental waters in presence of its natural constituents.

The accuracy and precision of the proposed kinetic method: The accuracy and precision of the proposed kinetic method was established by determining the content of Se at different concentration levels in spiked water (in the range of 2 - 20 µg L⁻¹) for the determination and speciation of Se. The results of the recoveries by using fixed time method along with standard error (SE) and standard deviation (SD) are presented in Table 4. The recoveries data presented are quite satisfactory. Thus, it can be expressed that the proposed kinetic method may be

very effective in the analysis of inorganic Se in water samples.

The analytical applications of the proposed kinetic method:

In order to evaluate the analytical applicability of the proposed method it was applied to the determination of selenium in natural water samples. The water samples were collected and filtered and their selenium contents were measured by the proposed method after removing the cationic interference species with Amberlite IR120 plus (Table 5). As this table shows, the results of the recovery of added Se(IV) and Se(VI) were satisfactory. Additionally, the proposed method was applied to a standard reference material, NIST SRM 1643e "Trace Elements in Water", with a selenium content of 11.97 ± 0.14 µg L⁻¹. Mass concentrations of SRM 1643e were calculated using the measured density of 1.025 g mL⁻¹. Using the proposed method, the content of Se in this SRM was 11.92 ± 0.03 µg L⁻¹. A comparison using *t*-test, demonstrate that there is not significant difference among the achieved results using the proposed method and the certified values. By the other way, Certified Reference Material of River Water or Natural Water with certified values for Se(IV) and Se(VI) do not exist however, the method of standard addition is considered as a validation method,⁴⁵ therefore, increasing quantities of Se(IV) and Se(VI) were added to the river samples and Se(IV) and Se(VI) were determined by the proposed method (Table 5).

Conclusions

The developed kinetic method can be used to determine selenium at levels as low as 0.215 µg L⁻¹ without the need for any preconcentration step. This novel kinetic technique is suitable for the determination of the speciation of Se(IV) and Se(VI) in environmental samples either directly analyzing them or after removal of potential interfering cationic species using a strongly cation-exchange resin such as Amberlite IR120 plus when being necessary. The proposed method has the advantages of low cost, simple operation, a linear range of 35 fold, reproducibility, accuracy and, most importantly, low DLs, comparable with the DLs obtained by the existing catalytic kinetic techniques.²³⁻³⁶ As a result, the proposed kinetic method can be simply replaced by the use of common chromatographic and atomic spectroscopic method with speedy analysis in order to determine and speciate inorganic Se and Se species in a simple matrix such as environmental surface waters. In addition, kinetic methods available, especially for use in underdeveloped and developing countries in order to detect the selenium present in real life samples can routinely be utilized for a local laboratory.

Acknowledgments. Authors wish to express their gratitude to Professor Mehmet AKÇAY for all expertly discussions with him during his stay at University and were exchanged in a number of e-mails even after his departure, as all of his suggestions contributed enormously in the preparation of this manuscript.

References

- NeÁve, J.; Henry, M.; Peretz, A.; Mareschi, J. P. *Cah. Nutr. DieÁt.* **1987**, *22*, 145.
- Frost, D. V. *Crit. Rev. Toxicol.* **1972**, *467*.

3. El-Shahawi, M. S.; Othman, A. M.; Othman A. S.; El-Sonbati, M. A. *Int. J. Environ. Anal. Chem.* **2006**, *86*, 941-954.
4. D'Ulivo, A. *Analyst* **1997**, *122*, 117R-144R.
5. Capelo, J. L.; Fernandez, C.; Pedras, B.; Santos, P.; Gonzalez, P.; Vaz, C. *Talanta* **2005**, *68*, 1442-1447.
6. Saygi, K. O.; Melek, E.; Tuzen, M.; Soylak, M. *Talanta* **2007**, *71*, 1375-1381.
7. Oram, L. L.; Strawn, D. G.; Marcus, M. A.; Fakra, S. C.; Moller, G. *Environ. Sci. Technol.* **2008**, *42*, 6830-6836.
8. Tuzen, M.; Saygi, K. O.; Soylak, M. *Talanta* **2007**, *71*, 424-429.
9. Campanella, L.; Ferri, T.; Morabito, R. A. *Analysis* **1989**, *17*, 507.
10. Kumar, A. R.; Riyazuddin, P. *Int. J. Environ. Anal. Chem.* **2007**, *87*, 469-500.
11. de Souza, S. S.; Santos, D., Jr.; Krug, F. J.; Barbosa, F., Jr. *Talanta* **2007**, *73*, 451-457.
12. Zhang, L.; Morita, Y.; Sakuragawa, A.; Isozaki, A. *Talanta* **2007**, *72*, 723-729.
13. Rurikova, D.; Tothova, E. *Chem. Papers* **1999**, *53*, 26-33.
14. Sucharova, J.; Suchara, I. *Anal. Chim. Acta* **2006**, *576*, 163-176.
15. Wallschlager, D.; Roehl, R. *J. Anal. Atom. Spectr.* **2001**, *16*, 922-925.
16. El-Shahawi, M. S.; El-Sonbati, M. A. *Talanta* **2005**, *67*, 806-815.
17. Stripeikis, J.; Costa, P.; Tudino, M.; Troccoli, O. *Anal. Chim. Acta* **2000**, *408*, 191.
18. Naik, R. M.; Srivastava, A.; Prasad, S. *Spectrochim. Acta Pt. A: Mol. Biomol. Spectrosc.* **2008**, *69*, 193-197.
19. Naik, R. M.; Sarkar, J.; Prasad, S. *Microchem. J.* **2008**, *88*, 45-51.
20. Prasad, S. *Anal. Lett.* **2004**, *37*, 2851-2867.
21. Prasad, S. *J. Anal. Chem.* **2005**, *60*, 581-588.
22. Prasad, S. *Microchem. J.* **2007**, *85*, 214-221.
23. Martinez Lozano, C.; Perez Ruiz, T.; Tomas, V.; Abellan, C. *Analyst* **1989**, *114*, 715.
24. Gökmen, I. G.; Abdelkader, E. *Analyst* **1994**, *119*, 703.
25. Ensafi, A. A.; Bagherian Dehaghi, G. *Anal. Lett.* **1995**, *28*(2), 335-347.
26. Safavi, A.; Afkhami, A. *Anal. Lett.* **1995**, *28*, 1095.
27. Safavi, A.; Sedghi, H. R.; Shams, E. *Fresenius J. Anal. Chem.* **1999**, *365*, 504.
28. Afkhami, A.; Madrakian, T. *Talanta* **2002**, *58*, 311-317.
29. Songsasen, A.; Aukkarayunyong, P.; Bangkedphol, S.; Sasomsap, W. *Kasetsart J. Nat. Sci.* **2002**, *36*, 103-109.
30. Gurkan, R.; Akcay, M. *Microchem. J.* **2003**, *75*, 39-49.
31. Ensafi, A. A.; Lemraski, M. S. *Anal. Lett.* **2004**, *37*, 2469-2483.
32. Nakano, S.; Yoshii, M.; Kawashima, T. *Talanta* **2004**, *64*, 1266-1272.
33. Gudzenko, L. V.; Pantaler, R. P.; Blank, A. B. *J. Anal. Chem.* **2004**, *59*, 935-938.
34. Zhengjun, G.; Xinshen, Z.; Guohe, C.; Xinfeng, X. *Talanta* **2005**, *66*, 1012-1017.
35. Keyvanfard, M.; Sharifian, A. *J. Anal. Chem.* **2006**, *61*, 596-600.
36. Chand, V.; Prasad, S. *J. Hazardous Mater.* **2009**, *165*(1-3), 780-788.
37. Brimmer, P.; Fawcett, W.; Kulhavy, A. *Anal. Chem.* **1987**, *59*, 1470-1471.
38. Afkhami, A.; Madrakian, T. *Talanta* **2002**, *58*, 311-317.
39. Safavi, A.; Absalan, G.; Maesum, S. *Anal. Chim. Acta* **2001**, *432*, 229-233.
40. Linares, P.; Castro, L. D.; Valcarcel, M. *Analyst* **1986**, *111*, 1405-1407.
41. Afkhami, A.; Afshar-E-Asl, A. *Anal. Chim. Acta* **2000**, *419*, 101-106.
42. Afkhami, A.; Mosaed, F. *Anal. Sci.* **2002**, *18*, 667-670.
43. Prasad, S. *Anal. Chim. Acta* **2005**, *540*, 173-180.
44. Pais, I.; Jones, B. J., Jr. *The Handbook of Trace Elements*; St. Louis Press: 1997; Florida.
45. Pichard, E.; MacKay, G. M.; Pionts, J. *Trace Analysis: A Structured Approach to Obtaining Reliable Results*; the Royal Society of Chemistry: 1996; UK, p 38.