



# Verification of a computer-aided replica technique for evaluating prosthesis adaptation using statistical agreement analysis

Hang-Nga Mai<sup>1</sup>, Kyeong Eun Lee<sup>2</sup>, Kyu-Bok Lee<sup>3</sup>, Seung-Mi Jeong<sup>4</sup>, Seok-Jae Lee<sup>5</sup>, Cheong-Hee Lee<sup>6</sup>, Seo-Young An<sup>7</sup>, Du-Hyeong Lee<sup>6\*</sup>

<sup>1</sup>Department of Prosthodontics, School of Dentistry, Kyungpook National University, Daegu, Republic of Korea; and Department of Prosthodontics, National Hospital of Odonto-Stomatology, Hanoi, Vietnam

<sup>2</sup>Department of Statistics, Kyungpook National University, Daegu, Republic of Korea

<sup>3</sup>Department of Prosthodontics, School of Dentistry, A3DI, Kyungpook National University, Daegu, Republic of Korea

<sup>4</sup>Department of Dentistry, Yonsei University Wonju College of Medicine, Wonju, Republic of Korea

<sup>5</sup>Department of Production Engineering, School of Mechanical Engineering, Kyungpook National University, Daegu, Republic of Korea

<sup>6</sup>Department of Prosthodontics, School of Dentistry, Kyungpook National University, Daegu, Republic of Korea

<sup>7</sup>Department of Oral and Maxillofacial Radiology, School of Dentistry, Kyungpook National University, Daegu, Korea

**PURPOSE.** The purpose of this study was to evaluate the reliability of computer-aided replica technique (CART) by calculating its agreement with the replica technique (RT), using statistical agreement analysis. **MATERIALS AND METHODS.** A prepared metal die and a metal crown were fabricated. The gap between the restoration and abutment was replicated using silicone indicator paste (n = 25). Gap measurements differed in the control (RT) and experimental (CART) groups. In the RT group, the silicone replica was manually sectioned, and the marginal and occlusal gaps were measured using a microscope. In the CART group, the gap was digitized using optical scanning and image superimposition, and the gaps were measured using a software program. The agreement between the measurement techniques was evaluated by using the 95% Bland-Altman limits of agreement and concordance correlation coefficients (CCC). The least acceptable CCC was 0.90. **RESULTS.** The RT and CART groups showed linear association, with a strong positive correlation in gap measurements, but without significant differences. The 95% limits of agreement between the paired gap measurements were 3.84% and 7.08% of the mean. The lower 95% confidence limits of CCC were 0.9676 and 0.9188 for the marginal and occlusal gap measurements, respectively, and the values were greater than the allowed limit. **CONCLUSION.** The CART is a reliable digital approach for evaluating the fit accuracy of fixed dental prostheses. [*J Adv Prosthodont* 2017;9:358-63]

**KEYWORDS:** Computer-aided replica technique; Concordance correlation coefficient analysis; Prosthesis adaptation; Reliability; Verification; Silicone replica technique

Corresponding author:  
Du-Hyeong Lee

Department of Prosthodontics, School of Dentistry, Kyungpook National University, 2175 Dalgubeoldae-ro, Jung-gu, Daegu 06130, Republic of Korea

Tel. +82536007676; e-mail, deweylee@knu.ac.kr

Received November 2, 2016 / Last Revision February 3, 2017 / Accepted March 21, 2017

© 2017 The Korean Academy of Prosthodontics

This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

This research was supported by Basic Science Research Program through the National Research Foundation of Korea(NRF) funded by the Ministry of Science, ICT & Future Planning(NRF-2014R1A1A1006073).

## INTRODUCTION

Accurate fit is essential for the success and longevity of dental prostheses.<sup>1</sup> Inadequate marginal or internal fit may lead to cement dissolution and plaque accumulation, thereby increasing the risks of dental caries, endodontic inflammation, and periodontitis.<sup>2,3</sup> Various methods have been used for the measurement of the level of adaptation of prostheses.<sup>4,6</sup> The silicone replica technique (RT) is a widely used and acceptable method for measuring the gap between the prostheses and abutment.<sup>7-9</sup> The gap is replicated using impression silicone and then measured by microscopy at the marginal and internal regions. Since the measurement is performed using the replica, the technique can be applied in

both *in vivo* and *ex vivo* studies. The procedure of RT mimics the clinical cementation process, thereby increasing clinical relevance.<sup>10</sup> Moreover, this technique allows evaluation of the internal fit of prostheses, such as in the axial and occlusal regions. The accuracy and reliability of RT have been verified in previous studies.<sup>9-11</sup> Laurent *et al.*<sup>10</sup> reported that the use of RT allowed accurate prediction of the fit of prostheses, regardless of the measurement location. Similarly, Rahme *et al.*<sup>11</sup> concluded that the RT was highly accurate and reliable in reproducing the thickness of cementation space. However, this technique is based on a 2-dimensional analysis and is prone to error during silicone sectioning and measurement.<sup>12,13</sup> To decrease methodological errors and obtain 3-dimensional data, the computer-aided replica technique (CART) has been proposed.<sup>14,15</sup> This digital approach used an optical scanning and image-superimposition process to digitize the gap space. This approach facilitates not only visualization of the gap, but also allows 3-dimensional geometric analysis.

Measurement of agreement is required to prove the acceptability of a new method or process before its application.<sup>16,17</sup> Several statistical methods, such as the Pearson's correlation coefficient, intraclass correlation coefficient, within-subject coefficient of variation, and concordance correlation coefficient (CCC), can be used to verify the agreement.<sup>18</sup> The CCC was first proposed by Lin in 1989.<sup>19</sup> This method identifies the agreement between two methods by calculating variations in their linear relationship from the 45 degrees line running through the origin. The advantage of CCC is that the indices reveal the accuracy and precision level as well as the degree of agreement.<sup>17,20</sup> For accuracy measurement, the distance from the best-fit line to the concordance line is evaluated, and for precision measurement, deviation of the observations from the best-fit linear line is evaluated. The agreement is determined on a scale of 1 (perfect agreement) to 0 (no agreement) to -1 (perfect reversed agreement).<sup>21</sup> It was previously reported that the CCC is an effective means for verifying a new method. Cerna *et al.*<sup>22</sup> showed the efficacy of this verification method for determining the reliability of a new occlusal analyzer for measuring bite force. The CCC is also widely used for calculating sample size for validation studies, generalizing linear and nonlinear mixed-effects models by assessing the fit, and improving the ability of estimating data with outliers.<sup>21,23,24</sup>

Although the recently developed CART is a useful method for analyzing the adaptation of fixed prostheses 3-dimensionally, the validity of this method has not been proven. The purpose of this study was to verify the CART by calculating its level of agreement with RT using the CCC statistical method.

## MATERIALS AND METHODS

A prepared premolar with a 1.0-mm deep chamfer margin and total convergence angle of 6 degrees<sup>25</sup> was designed in dedicated software (CATIA V5 R18; Dassault Systemes, Suresnes Cedex, France). The die design contained the base

part, with notches. The virtual die was imported into CAD software (Ceramill match2; Amann Girrbach, Koblach, Austria) to design a crown. The cementation space of the crown was set at 50  $\mu\text{m}$ , starting 1.0 mm above the margin.<sup>26</sup> Thereafter, the designs were processed to the metal die and crown by using a millable cobalt-chromium block (Ceramill Sintron; Amann Girrbach, Koblach, Austria) and a 5-axis milling machine (Ceramill Motion 2; Amann Girrbach, Koblach, Austria) (Fig. 1).


The surface texture of the metal die was modified to a matte surface by using airborne-particle abrasion, using alumina oxide of a 50- $\mu\text{m}$  particle size, at a pressure of 2.8 bar, for 12 seconds, from a distance of 10 mm, in order to decrease light reflection. Then, it was digitized using an optical scanner (Ceramill Map 400; Amann Girrbach, Koblach, Austria), and the surface image was saved in Standard Tessellation Language (STL) format (STL-A). The intaglio of the crown was filled with a silicone indicator paste (Fit Checker II; GC, Tokyo, Japan). Then, the crown was placed on the metal die under a static loading pressure of 50 N, in the direction of the long axis of the die, for 10 minutes.<sup>14</sup> The crown was carefully removed, leaving a silicone layer on the metal die (Fig. 2). The silicone layer and base part of the die were scanned and saved in STL format (STL-B). Using these procedures, a total of 25 silicone replicas and scanning sets were prepared.



Fig. 1. Metal die and crown.



Fig. 2. Silicone replica on metal die.

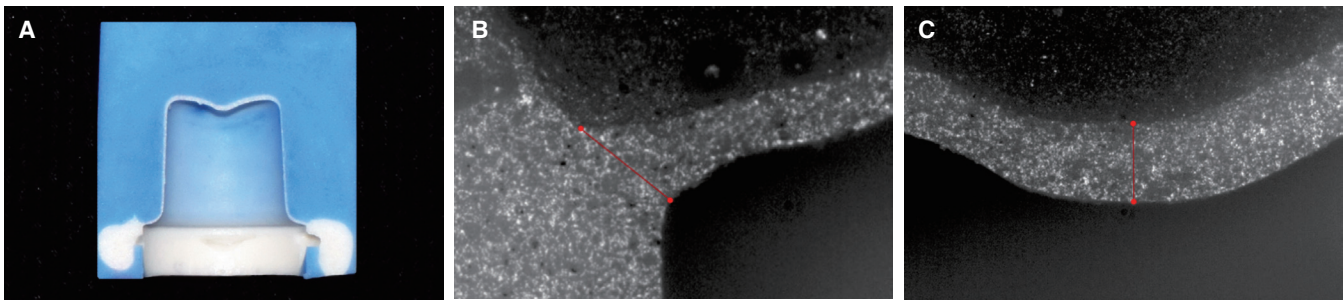

**Fig. 3.** Fit evaluation in replica technique. (A) Manual sectioning of silicone replica on the buccolingual plane, (B) Marginal gap measurement using microscope, (C) Occlusal gap measurement using a microscope.



**Fig. 4.** Fit evaluation in computer-aided replica technique. (A) Digital sectioning of 3D image of gap space in the buccolingual plane, (B) Marginal gap measurement using a software program, (C) Occlusal gap measurement using software program.

Two different methods, RT and CART, were used to evaluate the fit accuracy of the crown. For the RT group, a heavy body silicone (Virtual; Ivoclar Vivadent, Schaan, Liechtenstein) was applied over the gap space silicone replica for stabilization. Subsequently, the silicone block was perpendicularly sectioned along the buccolingual plane at the centric long axis of the tooth by using a razor blade (Personna; American Safety Razor, Verona, Virginia, USA) (Fig. 3A), and observed using a measuring microscope (Nikon MM-40; Nikon, Tokyo, Japan) under  $\times 50$  magnification (Fig. 3B, Fig. 3C). For the CART group, the STL-A and STL-B files were imported to a software program for 3D image analysis (Geomagic DesignX; 3D Systems Inc., Rock Hill, SC, USA). The two STL files were superimposed using the congruent base part of the die, and then the gap space was extracted by subtracting the STL-A from the STL-B.<sup>15</sup> The 3D image of the gap space was vertically sectioned at the center of the image, at which a cross-sectional contour line image was obtained (Fig. 4A). In the cross-sectional image, the gaps between the restoration and abutment were automatically measured by marking points on the contour line (Fig. 4B, Fig. 4C). The fit accuracy was evaluated in the marginal and occlusal regions. The marginal gap was defined as the distance between the most external point of the crown margin and the die finish line, while the occlusal gap was defined as the vertical distance between the crown and die at the center fossa region.<sup>1</sup> One operator, who was blinded to the purpose of this study, performed all measurements.

The reliability of gap measurement was then evaluated using CCC, the Bland-Altman method for each of RT and CART pair. The CCC value ( $\rho_c$ ) was computed as follow using statistical package R, version 3.2.5 (R Core Team, Vienna, Austria):<sup>16,19</sup>

$$\rho_c = 1 - \frac{\text{ratio of the mean square of within sample total deviation and the total deviation}}{2 \times \sigma_x \times \sigma_y} = \frac{2 \times \sigma_x \times \sigma_y}{\sigma_x^2 + \sigma_y^2 + (\mu_x - \mu_y)^2}$$

where  $\sigma_x^2$  and  $\sigma_y^2$  are the variances for the two variables,  $\mu_x$  and  $\mu_y$  and are the corresponding means.

The agreement was defined as follows: the within-sample total deviation was not more than 31.6% of the total deviation.<sup>9</sup> This translates into a least-acceptable CCC of 0.90 (1-0.316<sup>2</sup>). Lower 95% confidence limits were obtained from the bootstrap percentile using a fixed, large number of bootstrap resamples.

When the agreement measurement shows evidence of disagreement, the sources of the discrepancies should be addressed. It is necessary to determine whether the discrepancy is due to a shift in marginal distribution (inaccuracy) or due to a large within-sample variation (imprecision). The accuracy coefficient ( $\alpha_a$ ) is:<sup>16</sup>

$$\alpha_a = \frac{2}{\omega + \frac{1}{\omega} + \theta^2}$$

where  $\omega = \frac{\sigma_x}{\sigma_y}$  and  $\theta^2 = \frac{(\mu_x - \mu_y)^2}{\sigma_x \times \sigma_y}$ .

The precision coefficient ( $\rho$ ) was drawn using the CCC ( $\rho_c$ ) and accuracy coefficient ( $x_a$ ) as below.<sup>16</sup>

$$\rho = \frac{\rho_c}{x_a}$$


The Bland-Altman method presented the magnitude of differences in the gap measurements by obtaining the 95% limits of agreement between the gap measurements.<sup>27</sup> The Bland-Altman plots were drawn using MATLAB software (MathWorks Inc., Natick, MA, USA) where X axis was the mean of two paired measurements and Y axis was the relative difference between two paired measurements.<sup>27</sup>

## RESULTS


The two methods showed a linear association, with a strong positive correlation in the gap measurements (Fig. 5). The data points were clustered around the 45-degree line, with

little variation. The 95% limits of agreement range between the gaps measured by the RT and the CART were 3.84% and 7.08%, respectively, of the mean for the marginal and occlusal gap measurements (Fig. 6). The relative deviations were smaller in the marginal region than in the occlusal region.

Table 1 and Table 2 show the agreement statistics for the marginal and occlusal gap measurements. The CCC estimates and one-sided lower 95% confidence limits were greater than the allowance level for both regions. A value exceeding 0.91 was considered to represent good agreement. The accuracy and precision estimates for the marginal gap were 0.9999 and 0.9838, respectively, while these values for the occlusal gap were 0.9805 and 0.9726, respectively. In both these regions, the accuracy estimates were greater than the precision estimates. The lower 95% confidence limits showed similar tendencies to these estimates.

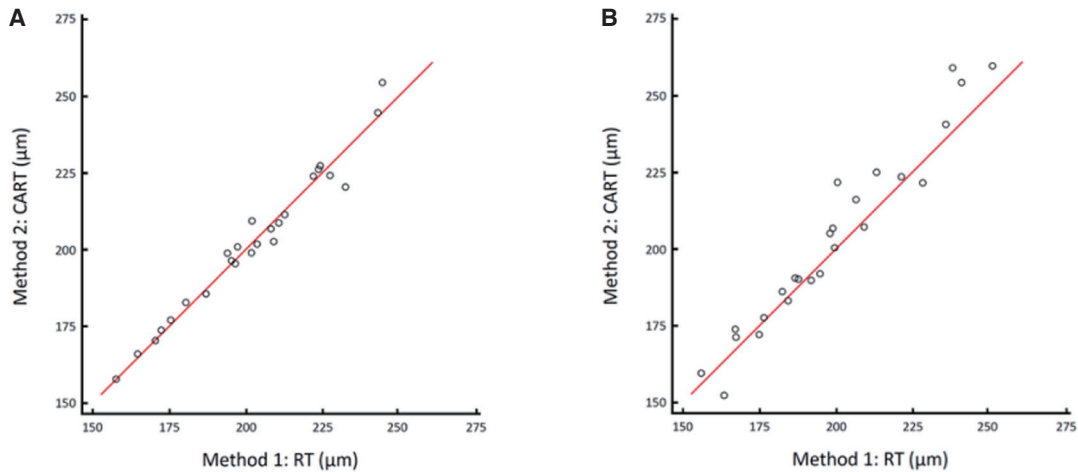

**Fig. 5.** Scatter plots of replica technique and computer-aided replica technique. (A) Marginal gap, (B) Occlusal gap. The red line represents a 45-degree line.

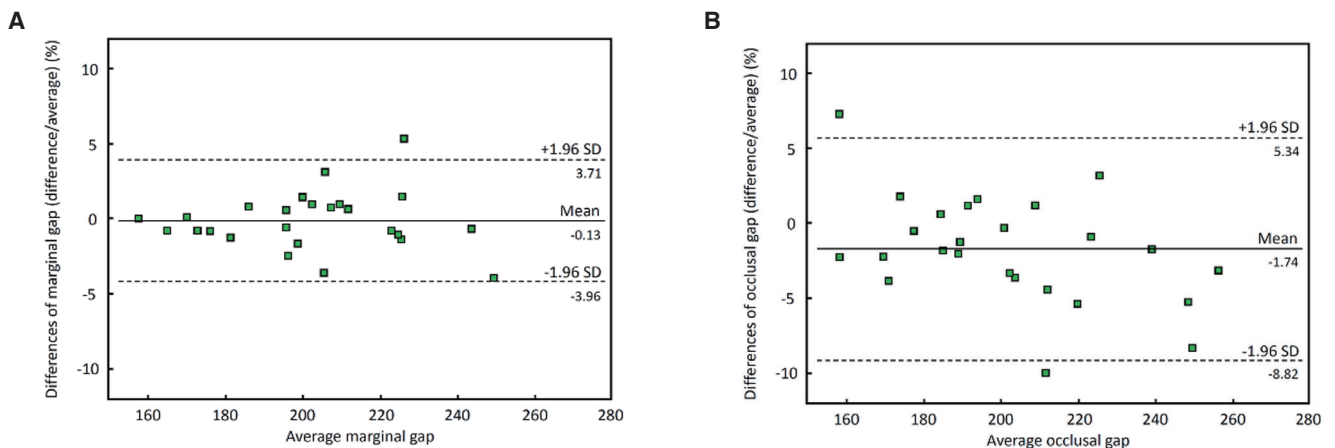

**Fig. 6.** Bland-Altman plots for reliability of gap measurements. (A) Marginal gap, (B) Occlusal gap.

**Table 1.** Agreement statistics and their confidence limits in the marginal gap measurements

Statistics	Estimate	Lower 95% confidence limit	Allowance
CCC	0.9837	0.9676	0.90
Accuracy	0.9999	0.9945	
Precision	0.9838	0.9700	

\*CCC: Concordance correlation coefficient.

The X-axes show the means of gaps measured using both techniques, and the Y-axes show differences between gaps in each pair as a percentage of their mean. Solid lines = mean absolute differences. Dashed lines = 95% limits of agreement.

## DISCUSSION

This study accessed the validity of the CART for evaluating the fit accuracy of fixed dental prostheses by using statistical agreement analysis and confirmed that the measurement value obtained from the CART agreed with that of the RT, with high accuracy and adequate precision. Thus, based on the results of this study, it is conceivable that the CART is a feasible method for 3-dimensional analysis of fixed dental prostheses.

The advantages of converting a gap space to a virtual image include the convenient data handling and increased data utilization. Since the measurement object is a digital image, outcome parameter analysis can be performed with ease by using the editing and measurement functions of computer software. This computer-aided approach allows various geometric analyses, such as the overall mean discrepancy, quantification of discrepancy in a specific region, and the entire volume of the gap space. A 3-dimensional, color-coded map showing discrepancies is also a useful way to reveal the distribution and degree of error.<sup>14,27,28</sup> Another advantage of digitization is the decrease in the possible error sources in methodology. The CART eliminates the manual replica sectioning process and reduces the need for decision-making during the selection of measurement points. Thus, this computer-aided approach could aid in obtaining more reliable results.

An indispensable prerequisite for use of the CART is to have a congruent area for image-superimposition of STL files. Without such a suitable reference area, high-quality image alignment cannot be performed. In this *in vitro* study, large and notch-including base parts of the die were used as a reference for superimposition. For clinical conditions, adjacent teeth or non-movable mucosa can be used as the reference area. Additionally, it is necessary to use a suitable optical scanner for the CART. Contemporary certified optical scanners show high accuracy and reproducibility.<sup>4</sup>

**Table 2.** Agreement statistics and their confidence limits in the occlusal gap measurements

Statistics	Estimate	Lower 95% confidence limit	Allowance
CCC	0.9537	0.9188	0.90
Accuracy	0.9805	0.9560	
Precision	0.9726	0.9511	

\*CCC: Concordance correlation coefficient.

Further large-sized clinical prospective trials are required to confirm the results of the present study and to evaluate the feasibility of applying it to various clinical conditions.

## CONCLUSION

Within the limitations of this statistical agreement study, it is confirmed that CART is as accurate as the RT for evaluating the fitness of fixed dental prostheses. Therefore, this digital approach can be applied to the analysis of fit accuracy of fixed dental prostheses for visualizing and quantifying the fit discrepancy 3-dimensionally.

## ORCID

Hang-Nga Mai <https://orcid.org/0000-0002-9832-3312>  
 Kyu-Bok Lee <https://orcid.org/0000-0002-1838-7229>  
 Seung-Mi Jeong <https://orcid.org/0000-0002-1543-7227>  
 Du-Hyeong Lee <https://orcid.org/0000-0003-2803-7457>  
 Seo-Young An <https://orcid.org/0000-0001-6711-5986>

## REFERENCES

- Holmes JR, Bayne SC, Holland GA, Sulik WD. Considerations in measurement of marginal fit. *J Prosthet Dent* 1989;62:405-8.
- Pimenta MA, Frasca LC, Lopes R, Rivaldo E. Evaluation of marginal and internal fit of ceramic and metallic crown copings using x-ray microtomography (micro-CT) technology. *J Prosthet Dent* 2015;114:223-8.
- Contrepois M, Soenen A, Bartala M, Laviolle O. Marginal adaptation of ceramic crowns: a systematic review. *J Prosthet Dent* 2013;110:447-54.
- Boitelle P, Mawussi B, Tapie L, Fromentin O. A systematic review of CAD/CAM fit restoration evaluations. *J Oral Rehabil* 2014;41:853-74.
- Torabi K, Vojdani M, Giti R, Taghva M, Pardis S. The effect of various veneering techniques on the marginal fit of zirconia copings. *J Adv Prosthodont* 2015;7:233-9.
- Ji MK, Park JH, Park SW, Yun KD, Oh GJ, Lim HP. Evaluation of marginal fit of 2 CAD-CAM anatomic contour zirconia crown systems and lithium disilicate glass-ceramic crown. *J Adv Prosthodont* 2015;7:271-7.

7. Bugurman BB, Turker SB. Clinical gap changes after porcelain firing cycles of zirconia fixed dentures. *J Adv Prosthodont* 2014;6:177-84.
8. Lee WS, Kim WC, Kim HY, Kim WT, Kim JH. Evaluation of different approaches for using a laser scanner in digitization of dental impressions. *J Adv Prosthodont* 2014;6:22-9.
9. Falk A, Vult von Steyern P, Fransson H, Thorén MM. Reliability of the impression replica technique. *Int J Prosthodont* 2015; 28:179-80.
10. Laurent M, Scheer P, Dejou J, Laborde G. Clinical evaluation of the marginal fit of cast crowns-validation of the silicone replica method. *J Oral Rehabil* 2008;35:116-22.
11. Rahme HY, Tehini GE, Adib SM, Ardo AS, Rifai KT. In vitro evaluation of the "replica technique" in the measurement of the fit of Procera crowns. *J Contemp Dent Pract* 2008;9:25-32.
12. Coli P, Karlsson S. Fit of a new pressure-sintered zirconium dioxide coping. *Int J Prosthodont* 2004;17:59-64.
13. Chan DC, Blackman R, Kaiser DA, Chung K. The effect of sprue design on the marginal accuracy of titanium castings. *J Oral Rehabil* 1998;25:424-9.
14. Kim KB, Kim JH, Kim WC, Kim JH. Three-dimensional evaluation of gaps associated with fixed dental prostheses fabricated with new technologies. *J Prosthet Dent* 2014;112: 1432-6.
15. Lee DH. Digital approach to assessing the 3-dimensional misfit of fixed dental prostheses. *J Prosthet Dent* 2016;116:836-839.
16. Lin L, Hedayat AS, Sinha B, Yang M. Statistical methods in assessing agreement: Models, issues, and tools. *J Am Stat Assoc* 2002;97:257-70.
17. Barnhart HX, Haber M, Song J. Overall concordance correlation coefficient for evaluating agreement among multiple observers. *Biometrics* 2002;58:1020-7.
18. Watson PF, Petrie A. Method agreement analysis: a review of correct methodology. *Theriogenology* 2010;73:1167-79.
19. Lin LI. A concordance correlation coefficient to evaluate reproducibility. *Biometrics* 1989;45:255-68.
20. King TS, Chinchilli VM, Wang KL, Carrasco JL. A class of repeated measures concordance correlation coefficients. *J Biopharm Stat* 2007;17:653-72.
21. Lawrence I, Lin K. Assay validation using the concordance correlation coefficient. *Biometrics* 1992;48:599-604.
22. Cerna M, Ferreira R, Zaror C, Navarro P, Sandoval P. Validity and reliability of the T-Scan<sup>®</sup> III for measuring force under laboratory conditions. *J Oral Rehabil* 2015;42:544-51.
23. King TS, Chinchilli VM. Robust estimators of the concordance correlation coefficient. *J Biopharm Stat* 2001;11:83-105.
24. Vonesh EF, Chinchilli VM, Pu K. Goodness-of-fit in generalized nonlinear mixed-effects models. *Biometrics* 1996;52:572-87.
25. Lopez-Suarez C, Gonzalo E, Pelaez J, Serrano B, Suarez MJ. Marginal vertical discrepancies of monolithic and veneered zirconia and metal-ceramic three-unit posterior fixed dental prostheses. *Int J Prosthodont* 2016;29:256-8.
26. Kokubo Y, Nagayama Y, Tsumita M, Ohkubo C, Fukushima S, Vult von Steyern P. Clinical marginal and internal gaps of In-Ceram crowns fabricated using the GN-I system. *J Oral Rehabil* 2005;32:753-8.
27. Giavarina D. Understanding bland altman analysis. *Biochem Med (Zagreb)* 2015;25:141-51.
28. Rhee YK, Huh YH, Cho LR, Park CJ. Comparison of intra-oral scanning and conventional impression techniques using 3-dimensional superimposition. *J Adv Prosthodont* 2015;7: 460-7.