



A new method to measure the accuracy of intraoral scanners along the complete dental arch: A pilot study

Mikel Iturrate^{1*}, Erlantz Lizundia^{2,3}, Xabier Amezua⁴, Eneko Solaberrieta⁴

¹Department of Business Management, Gipuzkoa Faculty of Engineering, University of the Basque Country UPV/EHU; Donostia - San Sebastián, Spain

²Department of Graphic Design and Engineering Projects, Bilbao Faculty of Engineering, University of the Basque Country UPV/EHU; Bilbao, Spain

³BCMaterials, Basque Center for Materials, Applications and Nanostructures, UPV/EHU; Leioa, Spain

⁴Department of Graphic Design and Engineering Projects, Gipuzkoa Faculty of Engineering, University of the Basque Country UPV/EHU; Donostia - San Sebastián, Spain

PURPOSE. The purpose of this study is to assess the accuracy of three intraoral scanners along the complete dental arch and evaluate the feasibility of the assessment methodology for further *in vivo* analysis. **MATERIALS AND METHODS.** A specific measurement pattern was fabricated and measured using a coordinate measuring machine for the assessment of control distances and angles. Afterwards, the pattern was placed and fixed in replica of an upper jaw for their subsequent scans (10 times) using 3 intraoral scanners, namely iTero Element1, Trios 3, and True Definition. 4 reference distances and 5 angles were measured and compared with the controls. Trueness and precision were assessed for each IOS: trueness, as the deviation of the measures from the control ones, while precision, as the dispersion of measurements in each reference parameter. These measurements were carried out using software for analyzing 3-dimensional data. Data analysis software was used for statistical and measurements analysis ($\alpha=.05$). **RESULTS.** Significant differences ($P<.05$) were found depending on the intraoral scanner used. Best trueness values were achieved with iTero Element1 (mean from $10 \pm 7 \mu\text{m}$ to $91 \pm 63 \mu\text{m}$) while the worst values were obtained with Trios3 (mean from $42 \pm 23 \mu\text{m}$ to $174 \pm 77 \mu\text{m}$). Trueness analysis in angle measurements, as well as precision analysis, did not show conclusive results. **CONCLUSION.** iTero Element1 was more accurate than the current versions of Trios3 and True Definition. Importantly, the proposed methodology is considered reliable for analyzing accuracy in any dental arch length and valid for assessing both trueness and precision in an *in vivo* study. [J Adv Prosthodont 2019;11:331-40]

KEYWORDS: Intraoral scanner; Accuracy; Trueness; Digital impression; Computer-aided design and computer-aided manufacturing (CAD/CAM)

Corresponding author:

Mikel Iturrate
Gipuzkoa Faculty of Engineering, UPV/EHU University of the Basque Country, Europa Plaza 1, 20.018 Donostia - San Sebastián, Spain
Tel. +34943018661; e-mail, mikel.iturrate@ehu.eus
Received July 10, 2019 / Last Revision October 8, 2019/ Accepted December 12, 2019

© 2019 The Korean Academy of Prosthodontics
This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/4.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

The work was partially supported by the Country Council of Gipuzkoa (Grant number 70/19).

INTRODUCTION

For intraoral scanners (IOS) to prevail over the conventional method, they must be easy-to-use and more efficient devices, and, especially, they must provide more accurate dental impressions for any restoration case. Accuracy is a requirement in any dental specialty, although it is certain that in some particular cases, the maximum allowable deviations are more restrictive. Prosthodontics is one of these specialties in which accuracy requirements are most demanding. This means that restorations fabricated from digital impressions must fit without causing any long-term clinical complications, i.e. with passive fit.¹ So far, the limits of the passive fit

have been analyzed in several studies, using different methodologies and measuring the admissible deviation in various directions.²⁻⁸

In dental implants, regardless of these limits, implant-supported reconstructions typically require a greater level of fit than teeth-supported reconstructions.⁹ Dental implants have reduced mobility and the lack of a periodontal ligament makes it impossible to adapt the implant to the poorly-adjusted framework; as a result, the implant and the framework are stressed.¹⁰ Accordingly, the goal of this work is to fabricate accurate restorations from digital impressions acquired with intraoral scanner (IOS). For that purpose, IOS must provide a reliable replica that will fit passively in the patient's mouth.

The development of IOS sought to overcome the challenges related to conventionally taken dental impressions, such as volumetric changes of impression materials, expansion of plaster models, or others related to the impression-taking process, such as improper tray selection, separation of impression material from the tray, or problems arising from the storage of impressions for the potential remaking of models.¹¹⁻¹³ By overcoming these challenges, within a few years IOS have increased their presence significantly.¹⁴ IOS and CAD/CAM already provide a more efficient way to perform restorations and have a higher acceptance rate among patients.¹⁵⁻²⁰

However, the practice of conventional impressions still persists. The validity of restorations made using IOS has been questioned from the beginning and many studies have been carried out to analyze their accuracy. Some have tried to directly assess the accuracy of IOS by performing studies *in vitro*.²¹⁻²⁶ Others have compared, also *in vitro*, digital impressions with conventional ones in larger areas such as a bridge or the complete arch^{11,15,27-30} or have compared conventionally or digitally-performed restorations.³¹⁻³⁸

All these studies have been performed using different methodologies, in varying lengths of arch, considering different conditions of the patient, such as edentulous or toothed, and even with different versions of the same IOS.^{24,39} These provided dentists and developers with varying results.

However, there is clearly a lack of accuracy studies performed *in vivo*. In this sense, when determining the accuracy of digital impressions, it is necessary to measure their trueness. The measurement of trueness has been the main obstacle in performing accuracy studies *in vivo*, even to the point of considering it impossible because of the difficulty to obtain references for trueness measurements.^{33-35,40}

The aim of this research was to design a new methodology that enables the study of the accuracy of digital impressions *in vivo* - a methodology based on the use of a pattern that allows the assessment of both trueness and precision in distance and angle measurements. Simultaneously, this methodology allows analysis of the accuracy in different lengths of dental arch. For this purpose, the methodology has been tested to assess the accuracy, in terms of trueness and precision, of three different IOS.

MATERIALS AND METHODS

The basis of the proposed methodology was to measure from digital impressions achieved with different IOS in a specifically designed pattern. This pattern was previously measured in a coordinate measuring machine (CMM) to obtain control distances and angles.

The pattern design had to meet three requirements: 1) the size and shape had to be suitable for replicating the study in different arch models; 2) the pattern had to be valid for measuring distance and angle errors along the complete arch; 3) the material had to be dimensionally stable and biocompatible to enable *in vivo* replication of the study if the methodology used was validated.

To fulfill the size and shape requirement, digital impressions of five upper jaws were used. The goal was to design a pattern that would fit in as many jaws as possible without interfering with dentition. For that purpose, five plaster models were randomly chosen and digitized with a blue light technology based industrial reference scanner (Camera resolution of $2 \times 5,000,000$ pixels and distance between points of 0.017 mm - 0.481 mm) (ATOS Compact Scan 5 M/300, GOM). From this digitization, five digital impressions in standard tessellation language (STL) were achieved. The jaws were completely dentate and without any diagnosed pathology. The five digital impressions of the upper jaws were aligned and overlapped using reverse engineering software (Geomagic Design X with 2016.2.2 software version) to define the space in which the designed pattern should fit. Then, the structure of the pattern was designed and five cylinders were digitally placed along the pattern in order to obtain useful geometries for both distance measurements and, using their axes, angle measurements. A reference plane was also machined as a base geometry for further measurements. The position of each cylinder corresponded approximately (depending on the characteristics of each jaw) to those of the maxillary right third molar, maxillary right canine, central maxillary incisors, maxillary left canine, and maxillary left third molar. Placing these reference cylinders

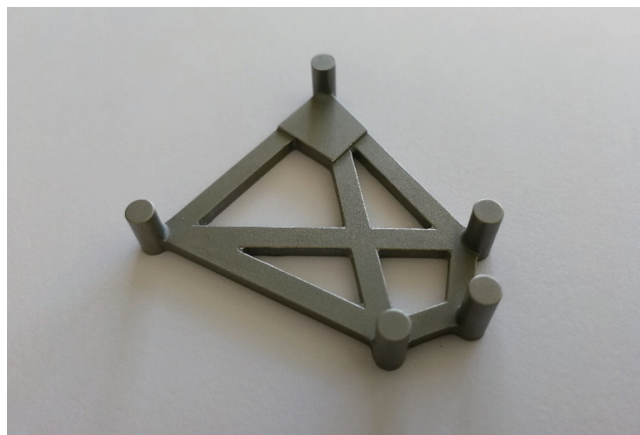


Fig. 1. Five reference cylinders in the fabricated stainless-steel pattern.

along the pattern allowed the measurement of the distance and angle error along the complete arch. Then, the reference pattern was designed and fabricated in stainless steel (Fig. 1). The surface of the pattern was shot-blasted to avoid glare and reflections that can interfere with the scanning process.

Four distances between the five cylinders and the angles of each cylinder were defined (D12, D13, D14, D15 and A1, A2, A3, A4, A5) for measurement and error analysis. Accuracy was evaluated in terms of trueness and precision. Trueness was assessed as the deviation of measured parameters (distance and angle) in IOS digital impressions from control ones and precision, as the deviation of each measurement of reference parameters in these digital impressions. In both cases, mean and standard deviation were calculated using statistical analysis software (IBM SPSS Statistics 24, IBM Corp., Armonk, NY, USA).

The pattern was placed and fixed on a plaster replica of the upper jaw using light-polymerizing resin (CONLIGHT, Kuss Dental, Madrid, Spain). Afterwards, the model with the pattern was scanned 10 times with each of the three selected IOS ($n = 30$): iTero Element1 (Hereafter iTero) (Align Technology Inc., San Jose, CA, USA) with 1.5.0.361 software version; Trios3, (3 Shape A/S) with 2015-1 software version; and True Definition (3M ESPE, St. Paul, MN, USA) with 5.1.1 software version. In all scans, the complete arch was digitized together with the five cylinders of the pattern (Fig. 2). All the scans were performed according to the IOS manufacturer's scanning protocols for complete arch. When the scans were performed with the iTero or Trios3, the scanning began in the maxillary right first molar, and when performed with the True Definition, the scanning began in the maxillary right canine. All scans ($n = 30$) were performed by the same technician, in the same clinic and under the same temperature and humidity conditions. The first scans were performed using the iTero and Trios3. Afterwards, when scanning with True Definition, the model with the pattern was powdered (Lava COS Powder, 3 M ESPE), as in clinical practice and following the manufacturer's recommendations.

The defined four distances and five angles of the pattern were measured first using a CMM (CRYSTA-Apex S, Mitutoyo) and assessed as control. These four distances and five angles were also measured from each digital impression obtained

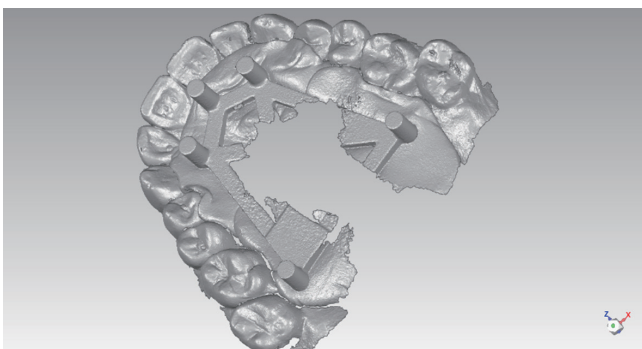


Fig. 2. The model combined with the digitized pattern.

with the IOS ($n = 30$) and compared with the controls. The measurements were performed using 3D inspection and mesh processing software for dimensional analysis (GOM Inspect with 2018 software version), following a specifically-designed measuring protocol.

To measure the 4 reference distances, 5 points were created in each cylinder of all STL files as the intersection between a cylinder axis and a plane. The reference distances were defined by linking these points (D12, D13, D14, and D15) (Fig. 3). The cylinders were created on each part of the mesh resembling a cylinder according to the Gaussian best-fit method. The software (GOM Inspect) squares the deviations of the selected polygons with the possible fitting element and adds the quadratic deviations. To create the intersection plane, firstly, the surface of the mesh corresponding to the horizontal plane of the pattern was selected taking into account only the mathematically useful surface of this horizontal area. The intersection plane was created as a 3 mm parallel plane to the previously created one.

Angles were measured using the axes of the created cylinders. The real angle between these axes and the plane created on the horizontal surface of the pattern was also measured.

Deviations were calculated as differences between the control reference distance and angles (measured using the CMM) and these reference parameters measured in digital impressions obtained with IOS.

Error in distance and angle measurements was measured in each of the reference parameters (reference distances and angles) and the mean and standard deviation of these errors were calculated. These calculations were repeated for each reference parameter and with each of the 3 IOS used. In addition, the results obtained with each IOS in each reference parameter were compared by applying the ANOVA variance analysis ($P < .05$). In order to apply this technique, the Levene test was previously used to check the homogeneity

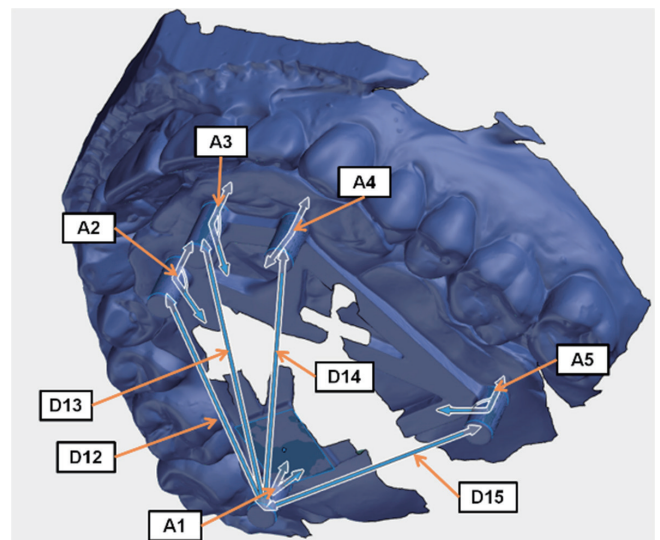


Fig. 3. Measured parameters in a digital impression of the upper jaw with the pattern included.

ty of the variances. Comparison of each measured parameter (distance and angle) was conducted using statistical analysis software (IBM SPSS Statistics 24, IBM Corp., Armonk, NY, USA).

RESULTS

After measuring the pattern with the CMM, reference distances were set at 32.405 mm for D12, 40.263 mm for D13, 40.622 mm for D14, and 32.804 mm for D15. Reference angles were set at 89°49'33" for A1, -89°53'48" for A2, -89°56'10" for A3, -89°55'50" for A4, and -89°51'59" for A5.

Concerning trueness, one-way ANOVA comparisons showed significant differences ($P < .05$) in all reference distances depending on the IOS used (Table 1). In order to discern the influence of each scanner, the scanners were compared in pairs, and results showed that these differences occurred especially when the Trios3 was involved. In all the distances that encompassed the equivalent of the digital impression of a quadrant including all incisors (D12, D13, and D14), significant differences were found comparing Trios3 with True Definition and Trios3 with iTero, while no significant differences were found between iTero and True Definition ($P = .522$ in D12, $P = .907$ in D13, and 0.764 in D14). In contrast, in D15 reference distance, the equivalent of a complete-arch digital impression, there were no significant differences comparing trueness achieved with Trios and True Definition ($P = .141$) or when comparing iTero with True Definition ($P = .412$). However, there were significant differences between Trios3 and iTero ($P = .014$).

Mean deviation ranged from $10 \pm 7 \mu\text{m}$ to $42 \pm 23 \mu\text{m}$ in D12 reference distance, from $16 \pm 9 \mu\text{m}$ to $69 \pm 34 \mu\text{m}$ in D13, from $21 \pm 22 \mu\text{m}$ to $109 \pm 44 \mu\text{m}$ in D14, and from 91

$\pm 63 \mu\text{m}$ to $174 \pm 77 \mu\text{m}$ in D15. In D12, D13, and D15 reference distances, best mean deviation values were achieved with iTero while the larger mean deviation values were achieved in all cases using Trios3. Table 1 summarizes deviation values obtained with each IOS in each reference distance.

Concerning precision, one-way ANOVA comparison did not show significant differences ($P > .05$) comparing the three IOS. Significant differences occurred only in D12 reference distance and between Trios3 and iTero ($P = .024$). Mean precision values ranged from $10 \pm 7 \mu\text{m}$ to $20 \pm 11 \mu\text{m}$ in D12 reference distance, from $14 \pm 13 \mu\text{m}$ to $28 \pm 18 \mu\text{m}$ in D13, from $16 \pm 18 \mu\text{m}$ to $33 \pm 27 \mu\text{m}$ in D14, and from $52 \pm 59 \mu\text{m}$ to $60 \pm 58 \mu\text{m}$ in D15 reference distance. Table 2 summarizes precision values obtained with each IOS in each reference distance.

Concerning the trueness of angle measurements, one-way ANOVA comparisons did not show significant differences ($P > .05$) among the three IOS (Table 3). Contrasting the scanners in pairs, in general, significant differences were found in each measured angle. Nonetheless, no significant differences were observed between Trios3 and iTero in A1 ($P = .874$) and A5 ($P = .660$) reference angle or between Trios3 and True Definition in A3 ($P = .103$) and A4 ($P = .668$) reference angles.

With regard to the measured angular deviations, it was found that while distance analysis clearly showed higher deviations as the scanning length increased, angle measurement analysis did not show the same evolution so clearly (Fig. 4). Minimum mean deviation values were measured in A1 reference angle ($0.082 \pm 0.068^\circ$); however, maximum mean deviation values were measured in A2 ($0.475 \pm 0.107^\circ$) and A3 ($0.484 \pm 0.127^\circ$) reference angles. All angle deviation values are shown in Table 3.

Table 1. Trueness in each reference distance and with each IOS

Reference Distance	IOS	Deviation (μm)			Levene P value	ANOVA F -value / P value
		Min. CI* (95%)	Max. CI* (95%)	Mean (SD)		
D12	iTero Element1	4	16	10 ± 7	$P = .244$	$f = 23.566$ $P = .000$
	Trios3	24	60	42 ± 23		
	True Definition	2	25	13 ± 14		
D13	iTero Element1	7	22	16 ± 9	$P = .216$	$f = 33.313$ $P = .000$
	Trios3	43	96	69 ± 34		
	True Definition	0	31	16 ± 19		
D14	iTero Element1	11	38	24 ± 17	$P = .333$	$f = 51.837$ $P = .000$
	Trios3	75	143	109 ± 44		
	True Definition	3	40	21 ± 22		
D15	iTero Element1	54	146	91 ± 63	$P = .828$	$f = 45.217$ $P = .000$
	Trios3	115	233	174 ± 77		
	True Definition	52	147	119 ± 86		

* CI: Confidence Interval

Table 2. Precision in each reference distance and with each IOS

Reference Distance	IOS	Precision (µm)			Levene <i>P</i> value	ANOVA F-value / <i>P</i> value
		Min. CI* (95%)	Max. CI* (95%)	Mean (SD)		
D12	iTero Element1	5	15	10 ± 7	<i>P</i> = .077	f = 0.032 <i>P</i> = .969
	Trios	11	28	20 ± 11		
	True Definition	4	22	12 ± 11		
D13	iTero Element1	8	22	16 ± 9	<i>P</i> = .092	f = 0.055 <i>P</i> = .947
	Trios	14	42	28 ± 18		
	True Definition	4	25	14 ± 13		
D14	iTero Element1	11	30	22 ± 13	<i>P</i> = .229	f = 0.024 <i>P</i> = .976
	Trios	12	54	33 ± 27		
	True Definition	3	32	16 ± 18		
D15	iTero Element1	35	71	55 ± 23	<i>P</i> = .921	f = 0.018 <i>P</i> = .982
	Trios	7	97	52 ± 59		
	True Definition	14	80	60 ± 58		

* CI: Confidence Interval

Table 3. Trueness in each reference angle and with each IOS

Reference Angle	IOS	Deviation (°)			Levene <i>P</i> value	ANOVA F-value / <i>P</i> value
		Min. CI* (95%)	Max. CI* (95%)	Mean (SD)		
A1	iTero Element1	0.083	0.263	0.184 ± 0.116	<i>P</i> = .674	f = 0.000 <i>P</i> = 1.000
	Trios3	0.080	0.272	0.176 ± 0.125		
	True Definition	0.030	0.140	0.082 ± 0.068		
A2	iTero Element1	0.077	0.178	0.121 ± 0.065	<i>P</i> = .174	f = 0.000 <i>P</i> = 1.000
	Trios3	0.393	0.558	0.475 ± 0.107		
	True Definition	0.262	0.468	0.339 ± 0.152		
A3	iTero Element1	0.057	0.139	0.099 ± 0.050	<i>P</i> = .081	f = 0.000 <i>P</i> = 1.000
	Trios3	0.387	0.582	0.484 ± 0.127		
	True Definition	0.306	0.508	0.377 ± 0.157		
A4	iTero Element1	0.074	0.178	0.117 ± 0.070	<i>P</i> = .034	f = 0.000 <i>P</i> = 1.000
	Trios3	0.253	0.438	0.345 ± 0.121		
	True Definition	0.235	0.575	0.38 ± 0.223		
A5	iTero Element1	0.129	0.359	0.239 ± 0.142	<i>P</i> = .505	f = 0.000 <i>P</i> = 1.000
	Trios3	0.071	0.345	0.208 ± 0.178		
	True Definition	0.263	0.618	0.439 ± 0.218		

* CI: Confidence Interval

Contrary to significant differences observed upon analyzing the trueness concerning angle measurement, with precision, in general no significant differences were found - only in A3 reference angle between Trios3 and iTero (*P* = .032), and in A3 and A4 between iTero and True Definition (*P* = .027 in both).

In line with angle trueness, precision measurements did not worsen as the scanning length increased (Fig. 4). Best precision values were obtained in A3 reference angle assessed on $0.042 \pm 0.024^\circ$ and obtained with iTero, and the least precise values were obtained in A5 and with True Definition, assessed on $0.169 \pm 0.126^\circ$ (Table 4).

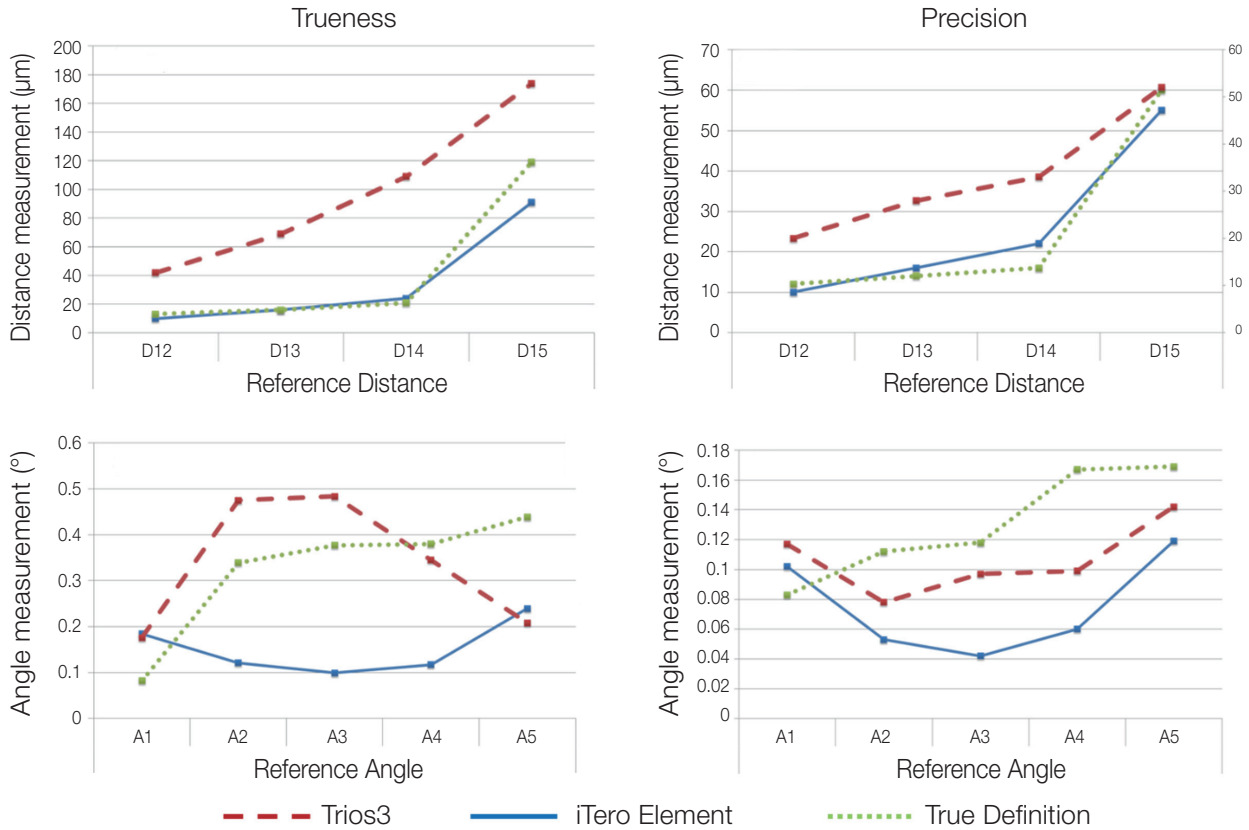


Fig. 4. Evolution of accuracy in terms of trueness and precision as the scanning length increases.

Table 4. Precision in each reference angle and with each IOS

Reference Angle	IOS	Precision (°)			Levene P value	ANOVA F-value / P value
		Min. CI* (95%)	Max. CI* (95%)	Mean (SD)		
A1	iTero Element1	0.041	0.162	0.102 ± 0.074	P = .674	f = 0.000 P = 1.000
	Trios3	0.084	0.150	0.117 ± 0.043		
	True definition	0.043	0.119	0.083 ± 0.047		
A2	iTero Element1	0.024	0.080	0.053 ± 0.034	P = .174	f = 0.000 P = 1.000
	Trios3	0.025	0.130	0.078 ± 0.068		
	True definition	0.029	0.167	0.112 ± 0.095		
A3	iTero Element1	0.028	0.060	0.042 ± 0.024	P = .081	f = 0.000 P = 1.000
	Trios3	0.039	0.154	0.097 ± 0.074		
	True definition	0.036	0.165	0.118 ± 0.096		
A4	iTero Element1	0.034	0.081	0.06 ± 0.03	P = .034	f = 0.000 P = 1.000
	Trios3	0.053	0.145	0.099 ± 0.06		
	True definition	0.050	0.271	0.167 ± 0.137		
A5	iTero Element1	0.077	0.177	0.119 ± 0.067	P = .505	f = 0.000 P = 1.000
	Trios3	0.069	0.215	0.142 ± 0.095		
	True definition	0.094	0.279	0.169 ± 0.126		

* CI: Confidence Interval

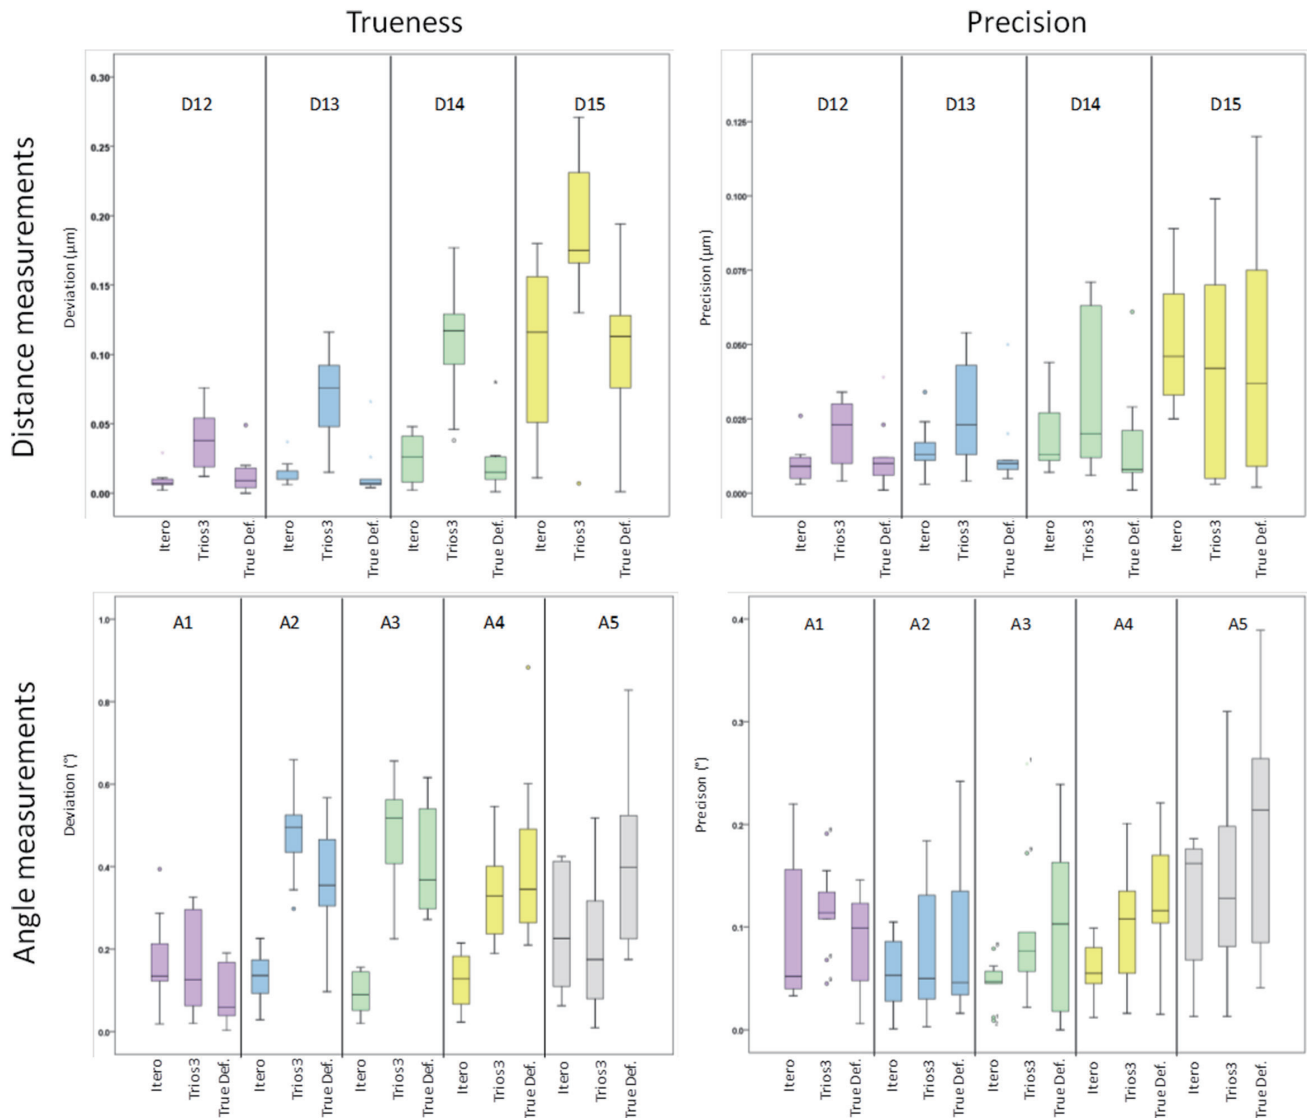


Fig. 5. Distribution of trueness and precision of each IOS in each reference distance and angle.

The distribution of trueness and precision data showed that distance error increased when the scanning area increased and that best results were achieved with iTero and True Definition (Fig. 5). Angle measurements did not show any conclusive data associated with the scanned arch length.

DISCUSSION

In this study, the accuracy of complete-arch digital impressions achieved with three intraoral scanners was assessed. The study was carried out following a new methodology and proved using *in vitro* tests.

The results obtained, similar to those obtained in previous studies, suggest that it is an applicable methodology for *in vivo* studies. This methodology was designed to measure

the accuracy of scanners and to analyze the validity of results in certain clinical practices such as the fabrication of complete or partial restorations.

Many studies calculated the accuracy of IOS by superimposing meshes obtained from these scanners, or with meshes obtained from industrial or desktop scanners.^{11,22,23,25,26,28,29} These superimpositions were carried out using best-fit alignment functions or minimizing distances criteria (specific functions to reverse engineering software). The results, obtained following these functions, provide important knowledge on the subject, especially for the manufacturers of scanners, although the use of scanners may present serious limitations in clinical practice when rehabilitations cover arch lengths longer than a dental piece.

The best fit functions align the meshes in order to achieve

the minimum error; thus, this error is distributed as homogeneously as possible throughout the whole mesh. When the whole mesh represents a reduced space of the dental arch (from one to two teeth), as in the case of an impression to prepare a crown, the measurements of the resultant distributed error can be useful to establish whether or not the dental digital impressions are accurate enough. Measured error using best fit alignment functions could resemble marginal fit errors. However, in rehabilitations with implant restorations, it is preferable to know the error between fixation points rather than the homogeneously distributed error. According to this criterion, mesh alignments should be performed aiming for zero error at the first fixation point and measuring the accumulated error at other fixation points, instead of using best fit alignment processes that distribute the error and minimize it in all the extension of the mesh. Some studies of IOS accuracy have followed these criteria of assessing distance or angulation errors between previously determined points.^{23,24,30,36,37}

The present study shows a methodology to assess the trueness and precision of digitally-acquired dental impressions using a measurement pattern. This pattern was provided with geometrically-helpful landmarks to easily measure the distance and angle errors, also used by other authors such as Van Deer Meer, Fukazawa, Güth, Zhang, or Kuhr.^{24,25,31,37,38}

On the other hand, many published IOS accuracy studies compared results achieved using IOS with results obtained by conventional procedures.^{11,15,27,28} However, these studies do not consider errors that conventional procedures can include. Impression materials can shrink, expand, or warp during or after removal from the mouth, resulting in inaccuracies. In addition, as in any type of process, each of the sub-processes carried out during conventional dental impressions can increase errors.¹¹⁻¹³ Therefore, one of the advantages of the proposed methodology is that instead of comparing the results with conventionally obtained models, they are compared with an accurately measured pattern that can be placed in the mouth. Thus, this methodology can be easily replicated in an *in vivo* study. Some studies have proposed similar methodologies based on the use of a pattern or externally-measured landmarks.^{30,37} However, the proposed methodology is valid for assessing the accuracy in different scanning lengths by measuring a once defined pattern. Thus, the deviation increase can be evaluated as the scanning length increases.

It is important to note that the proposed methodology has its limitations. The aim was to design a pattern that would fit in different mouths for later *in vivo* studies; for this, 5 volunteer arches were used. However, it is reasonable to assume that the pattern is not valid for all mouths and that in other cases the distances between the cylindrical abutments might not resemble implant or tooth positions. In addition, the shape of the pattern also limits the possibility of performing accuracy studies to the upper arch due to the difficulty of placing and maintaining the pattern placed in the lower arch. It is also worth noting that the study was performed using a pathology free and fully toothed model. The use of this same pattern in an edentulous case could influ-

ence the results since the pattern could provide the scanners with references to perform best fit unions. In addition to the obtained results, it should be noted that impression taking processes were performed using a model. It is assumed that the results presented would worsen in impressions *in vivo* due to the difficulties of obtaining them in real conditions.

In the trials conducted to test the methodology and establish the accuracy of IOS, distance and angle measurements showed different behaviors. Regarding distance analysis, results clearly showed that both trueness and precision worsened as the scanning area increased. These results also validate the proposed methodology for accuracy analysis as it confirms the conclusions obtained by previous studies (i.e. accuracy loss when increasing the length of dental arch to be scanned).^{11,28} As shown in Fig. 4, deviations measured from digital impressions achieved with True Definition and iTero are similar, particularly when the impression reaches an arch-quadrant, including the incisors. In this distance, both IOSs achieved mean deviations below 25 μm and the maximum at 40 μm (95% Confidence Interval). With the Trios3 scanner, the measured maximum deviations reached 143 μm (95% CI) in D14 while mean deviation was $109 \pm 44 \mu\text{m}$. Considering previous studies that set maximum permissible errors at 100 μm , only those results obtained with iTero and True in a quadrant including all incisors are considered acceptable.⁷ Others have set maximum admissible errors at 150 μm , which makes acceptable digital impressions of complete arch achieved with iTero and True Definition (mean deviation of $91 \pm 61 \mu\text{m}$ and $119 \pm 61 \mu\text{m}$ and maximum in CI 95% of 146 μm or 147 μm , respectively).¹⁷ The highest inaccuracies were measured with Trios3, reaching a mean deviation of $174 \pm 77 \mu\text{m}$ and a maximum of 233 μm (95% CI) in D14 distance.

The precision values showed a similar tendency to the deviations as shown in Fig. 4. Digital impressions were less precise as the scanning length of the arch increased, reaching values of maximum deviations in precision of 97 μm and 80 μm (Trios3 and True Definition in D15, respectively).

Angle measurement did not show such a clear trend due to the increase in the scanning arch length. However, Fig. 4 clearly shows how the best results in both trueness and precision were obtained with the iTero. The A1 and A5 reference angles did not give the best results despite there being no major differences among the scanners. However, in the angles A2, A3, and A4, the differences were greater and clearly showed better values for the iTero: deviation of $0.121 \pm 0.065^\circ$, $0.099 \pm 0.050^\circ$, and $0.117 \pm 0.070^\circ$ in A2, A3, and A4, respectively, and precision of $0.053 \pm 0.034^\circ$, $0.042 \pm 0.024^\circ$, $0.060 \pm 0.030^\circ$, and $0.119 \pm 0.067^\circ$ in A2, A3, A4, and A5, respectively. It is worth noting that all measured angles gave deviation values below 0.4° , proposed by Andriessen as the maximum permissible.⁶

Despite the limitations of this *in vitro* study, results showed that IOS provide accurate digital impressions of a quadrant, confirming the conclusions obtained by previously published works related to the improvements implemented by IOS manufacturers to these devices.^{24,39} Few years ago,

IOS were even discouraged for complete arch impressions and there were no studies measuring their accuracy at various arch lengths. However, the most recent studies, as well as the present one, measure the accuracy of the full arch. Results also validate the proposed methodology as the values obtained for both trueness and precision are close to the published studies on the subject. The evolution of the error measured along the length of the arch also indicates logical and expected results showing worsening tendencies when the digitized arch length increases.

CONCLUSION

The current study shows that, at the time of performing the experimental part, the latest version of iTero provided greater accuracy in digital impressions of a dentate dental arch than the latest versions of Trios3 and True Definition. In addition, the proposed methodology was considered reliable to assess accuracy in terms of trueness and precision *in vivo*, considering both distance and angle deviations and in any dental arch length.

ACKNOWLEDGEMENTS

The authors thank Dr Guillermo Pradies of the Complutense University of Madrid and Naiara Ortega of the Mechanics Department of the University of the Basque Country (UPV/EHU) for their support and assistance in the conduct of this research work.

ORCID

Mikel Iturrate <https://orcid.org/0000-0001-7113-7408>
 Erlantz Lizundia <https://orcid.org/0000-0003-4013-2721>
 Xabier Amezua <https://orcid.org/0000-0003-2163-9957>
 Eneko Solaberrieta <https://orcid.org/0000-0003-1734-2173>

REFERENCES

- Jemt T, Lie A. Accuracy of implant-supported prostheses in the edentulous jaw: analysis of precision of fit between cast gold-alloy frameworks and master casts by means of a three-dimensional photogrammetric technique. *Clin Oral Implants Res* 1995;6:172-80.
- Kan JY, Rungcharassaeng K, Bohsali K, Goodacre CJ, Lang BR. Clinical methods for evaluating implant framework fit. *J Prosthet Dent* 1999;81:7-13.
- Christensen GJ. Marginal fit of gold inlay castings. *J Prosthet Dent* 1966;16:297-305.
- Dedmon HW. Disparity in expert opinions on size of acceptable margin openings. *Oper Dent* 1982;7:97-101.
- Jemt T. Failures and complications in 391 consecutively inserted fixed prostheses supported by Brånemark implants in edentulous jaws: a study of treatment from the time of prosthesis placement to the first annual checkup. *Int J Oral Maxillofac Implants* 1991;6:270-6.
- Andriessen FS, Rijkens DR, van der Meer WJ, Wismeijer DW. Applicability and accuracy of an intraoral scanner for scanning multiple implants in edentulous mandibles: a pilot study. *J Prosthet Dent* 2014;111:186-94.
- Heckmann SM, Karl M, Wichmann MG, Winter W, Graef F, Taylor TD. Cement fixation and screw retention: parameters of passive fit. An in vitro study of three-unit implant-supported fixed partial dentures. *Clin Oral Implants Res* 2004;15:466-73.
- Vandeweghe S, Vervack V, Dierens M, De Bruyn H. Accuracy of digital impressions of multiple dental implants: an in vitro study. *Clin Oral Implants Res* 2017;28:648-653.
- Kim Y, Oh TJ, Misch CE, Wang HL. Occlusal considerations in implant therapy: clinical guidelines with biomechanical rationale. *Clin Oral Implants Res* 2005;16:26-35.
- Bacchi A, Consani RL, Mesquita MF, Dos Santos MB. Effect of framework material and vertical misfit on stress distribution in implant-supported partial prosthesis under load application: 3-D finite element analysis. *Acta Odontol Scand* 2013;71:1243-9.
- Patzelt SB, Emmanouilidi A, Stampf S, Strub JR, Att W. Accuracy of full-arch scans using intraoral scanners. *Clin Oral Investig* 2014;18:1687-94.
- Christensen GJ. Will digital impressions eliminate the current problems with conventional impressions? *J Am Dent Assoc* 2008;139:761-3.
- Christensen GJ. Impressions are changing: deciding on conventional, digital or digital plus in-office milling. *J Am Dent Assoc* 2009;140:1301-4.
- Richert R, Goujat A, Venet L, Viguie G, Viennot S, Robinson P, Farges JC, Fages M, Ducret M. Intraoral scanner technologies: A review to make a successful impression. *J Healthc Eng* 2017;2017:8427595.
- Ahrberg D, Lauer HC, Ahrberg M, Weigl P. Evaluation of fit and efficiency of CAD/CAM fabricated all-ceramic restorations based on direct and indirect digitalization: a double-blinded, randomized clinical trial. *Clin Oral Investig* 2016;20:291-300.
- Gjelvold B, Chrcanovic BR, Korduner EK, Collin-Bagewitz I, Kisch J. Intraoral digital impression technique compared to conventional impression technique. A randomized clinical trial. *J Prosthodont* 2016;25:282-7.
- Lee SJ, Gallucci GO. Digital vs. conventional implant impressions: efficiency outcomes. *Clin Oral Implants Res* 2013;24:111-5.
- Patzelt SB, Lamprinos C, Stampf S, Att W. The time efficiency of intraoral scanners: an in vitro comparative study. *J Am Dent Assoc* 2014;145:542-51.
- Gallardo YR, Bohner L, Tortamano P, Pigozzo MN, Laganá DC, Sesma N. Patient outcomes and procedure working time for digital versus conventional impressions: A systematic review. *J Prosthet Dent* 2018;119:214-9.
- Burhard L, Livas C, Kerdijsk W, van der Meer WJ, Ren Y. Treatment comfort, time perception, and preference for conventional and digital impression techniques: A comparative study in young patients. *Am J Orthod Dentofacial Orthop* 2016;150:261-7.
- Hack GD, Patzelt SB. Evaluation of the accuracy of six intra-

- oral scanning devices: An in-vitro investigation. *American Dent Assoc* 2015;10:1-5.
22. Omar Ali A. Accuracy of digital impressions achieved from five different digital impression system. *J Prosthodontics* 2015;5:2-6.
 23. van der Meer WJ, Andriessen FS, Wismeijer D, Ren Y. Application of intra-oral dental scanners in the digital workflow of implantology. *PLoS One* 2012;7:e43312.
 24. Fukazawa S, Odaira C, Kondo H. Investigation of accuracy and reproducibility of abutment position by intraoral scanners. *J Prosthodont Res* 2017;61:450-9.
 25. Güth JF, Runkel C, Beuer F, Stimmelmayer M, Edelhoff D, Keul C. Accuracy of five intraoral scanners compared to indirect digitalization. *Clin Oral Investig* 2017;21:1445-55.
 26. Imburgia M, Logozzo S, Hauschild U, Veronesi G, Mangano C, Mangano FG. Accuracy of four intraoral scanners in oral implantology: a comparative in vitro study. *BMC Oral Health* 2017;17:92.
 27. Patzelt SB, Bishri S, Stampf S, Att W. Accuracy of computer-aided design/computer-aided manufacturing-generated dental casts based on intraoral scanner data. *J Am Dent Assoc* 2014; 145:1133-40.
 28. Ender A, Mehl A. Accuracy of complete-arch dental impressions: a new method of measuring trueness and precision. *J Prosthet Dent* 2013;109:121-8.
 29. Ender A, Mehl A. In-vitro evaluation of the accuracy of conventional and digital methods of obtaining full-arch dental impressions. *Quintessence Int* 2015;46:9-17.
 30. Güth JF, Edelhoff D, Schweiger J, Keul C. A new method for the evaluation of the accuracy of full-arch digital impressions in vitro. *Clin Oral Investig* 2016;20:1487-94.
 31. Syrek A, Reich G, Ranftl D, Klein C, Cerny B, Brodesser J. Clinical evaluation of all-ceramic crowns fabricated from intraoral digital impressions based on the principle of active wavefront sampling. *J Dent* 2010;38:553-9.
 32. Zarauz C, Valverde A, Martinez-Rus F, Hassan B, Pradies G. Clinical evaluation comparing the fit of all-ceramic crowns obtained from silicone and digital intraoral impressions. *Clin Oral Investig* 2016;20:799-806.
 33. Ender A, Attin T, Mehl A. In vivo precision of conventional and digital methods of obtaining complete-arch dental impressions. *J Prosthet Dent* 2016;115:313-20.
 34. Ender A, Zimmermann M, Attin T, Mehl A. In vivo precision of conventional and digital methods for obtaining quadrant dental impressions. *Clin Oral Investig* 2016;20:1495-504.
 35. Zimmermann M, Koller C, Rumetsch M, Ender A, Mehl A. Precision of guided scanning procedures for full-arch digital impressions in vivo. *J Orofac Orthop* 2017;78:466-71.
 36. Zhang F, Suh KJ, Lee KM. Validity of intraoral scans compared with plaster models: An in-vivo comparison of dental measurements and 3D surface analysis. *PLoS One* 2016;11: e0157713.
 37. Kuhr F, Schmidt A, Rehmann P, Wöstmann B. A new method for assessing the accuracy of full arch impressions in patients. *J Dent* 2016;55:68-74.
 38. Nedelcu R, Olsson P, Nyström I, Rydén J, Thor A. Accuracy and precision of 3 intraoral scanners and accuracy of conventional impressions: A novel in vivo analysis method. *J Dent* 2018;69:110-8.
 39. Shim JS, Lee JS, Lee JY, Choi YJ, Shin SW, Ryu JJ. Effect of software version and parameter settings on the marginal and internal adaptation of crowns fabricated with the CAD/CAM system. *J Appl Oral Sci* 2015;23:515-22.
 40. Mangano F, Gandolfi A, Luongo G, Logozzo S. Intraoral scanners in dentistry: a review of the current literature. *BMC Oral Health* 2017;17:149.