

Effectiveness and Technical Considerations of Solitaire Platinum 4×40 mm Stent Retriever in Mechanical Thrombectomy with Solumbra Technique

Ho Jun Yi,^{1,2} Jae Hoon Sung,¹ Dong Hoon Lee,¹ Seung Yoon Song¹

Department of Neurosurgery,¹ St. Vincent's Hospital, College of Medicine, The Catholic University of Korea, Suwon, Korea
Department of Neurosurgery,² Hangang Sacred Heart Hospital, College of Medicine, Hallym University, Seoul, Korea

Objective : The Solitaire Platinum 4×40 mm stent retriever contains radiopaque markers with a long length. We evaluated the effect of Solitaire Platinum 4×40 mm stent retriever in Solumbra technique thrombectomy, and compared it with shorter Solitaire stent retrievers.

Methods : A total of 70 patients who underwent Solumbra technique thrombectomy with equal diameter (4 mm) and different length (40 vs. 20 mm) Solitaire stent retrievers were divided into two groups : the Solitaire Platinum 4×40 mm stent (4×40) group and the Solitaire FR 4×20 mm stent or Solitaire Platinum 4×20 mm stent (4×20) group. The clinical outcomes, Thrombolysis in Cerebral Infarction score, the first pass reperfusion status, and complications were evaluated and compared between the two groups. Multivariate analysis was performed to evaluate the predictive factors for reperfusion and complete reperfusion from the first pass.

Results : Higher first-pass reperfusion and complete reperfusion were achieved in the 4×40 group (68.0% and 48.0%) than in the 4×20 group (46.7% and 33.3%; $p=0.004$ and 0.007 , respectively). In multivariate analysis, radiopaque device and longer stent retriever were correlated with first-pass reperfusion ($p=0.014$ and 0.008 , respectively) and first-pass complete reperfusion ($p=0.022$ and 0.012 , respectively).

Conclusion : Our study demonstrated the usefulness of the Solitaire Platinum 4×40 mm stent retriever, which led to higher first-pass reperfusion and complete reperfusion rates than the Solitaire FR 4×20 mm stent or the Solitaire Platinum 4×20 mm stent, especially in Solumbra technique thrombectomy.

Key Words : Angiography · Reperfusion · Stents · Stroke · Thrombectomy.

INTRODUCTION

Mechanical thrombectomy (MT) is the primary modality for the treatment of acute ischemic stroke (AIS) caused by

large artery occlusion (LAO). In addition, the MT technique continues to evolve in terms of its effectiveness and diversity. Initially, the effectiveness of stent retriever techniques was demonstrated via several randomized controlled trials and

• Received : February 21, 2020 • Revised : March 30, 2020 • Accepted : April 1, 2020

• Address for reprints : **Jae Hoon Sung**

Department of Neurosurgery, St. Vincent's Hospital, College of Medicine, The Catholic University of Korea, 93 Jungbu-daero, Paldal-gu, Suwon 16247, Korea
Tel : +82-31-249-8985, Fax : +82-31-2649-7020, E-mail : jaehoonsung@gmail.com, ORCID : <https://orcid.org/0000-0003-3738-6413>

This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/4.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

meta-analyses, and the usefulness of contact aspiration technique was shown in several studies^{2,4,5,9,10,17,20,29,30}. In addition, a number of studies demonstrated that the chance of first-pass reperfusion was increased in Solumbra technique thrombectomy (stent retriever with simultaneous aspiration)^{8,16,21,22}.

Along with the evolution of MT techniques, devices for thrombectomy have also developed. The Solitaire AB stent (ev3; Covidien, Irvine, CA, USA) was the first stent-retriever device used in MT, and was developed further into the Solitaire flow restoration (FR) device and subsequently to the Solitaire 2 revascularization device. Solitaire is a nitinol stent retriever with laser-cut, attached to a push-wire with a closed-cell scaffolding design^{27,28}. However, the Solitaire FR stent retriever had a major disadvantage of poor visualization. The next generation Solitaire stent retriever, the Solitaire Platinum (Medtronic, Dublin, Ireland) has radiopaque platinum markers, which are spaced 10 mm apart. The use of a radiopaque device is known to be associated with first-pass reperfusion^{12,18}. In addition to the characteristics of the stent retriever, the size of the stent may affect the outcomes of MT. The appropriate stent diameter is disputed, and several reports suggested conflictingly, that a stent with a larger or smaller diameter was better^{13,31,33}. However, in terms of stent length rather than diameter, Haussen et al.¹² reported that longer stent retrievers enhance thrombectomy performance, probably due to the larger device-thrombus interaction area and smaller chances of missing the target site.

For these reasons, the authors used Solitaire Platinum 4×40 mm stent retriever with a Solumbra technique. Therefore, the purpose of our study was to assess the potential benefits of Solitaire Platinum 4×40 mm stent retriever with its radiopacity and long length, and compared it with other Solitaire stent retrievers, especially in patients who underwent MT with Solumbra technique. In addition, the technical considerations involved in Solumbra technique thrombectomy with Solitaire Platinum 4×40 mm stent retriever are also discussed.

MATERIALS AND METHODS

Study population

This retrospective study with prospectively collected data was approved by the Local Institutional Review Board (IRB No. VC17RESI0048) of each participating center. The data of

patients with LAO who underwent Solumbra technique thrombectomies with a Solitaire stent retriever of equal diameter (4 mm) between January 2018 and July 2019 were obtained from each institution's stroke database and evaluated. All of the procedures were performed by two experienced neuro-interventionalists at two centers. A total of 70 patients were identified for enrollment. These patients were dichotomized into : 1) a 4×40 group using 4×40 mm Solitaire stent retrievers (Solitaire Platinum 4×40 mm stent retriever) and 2) a 4×20 group using 4×20 mm Solitaire stent retrievers (Solitaire FR 4×20 mm or Solitaire Platinum 4×20 mm stent retrievers). Prior to thrombectomy, intravenous tissue plasminogen activator (IV t-PA, alteplase) was administered to patients within 4.5 hours after stroke onset at a maximum dose of 0.9 mg/kg in accordance with the European Cooperative Acute Stroke Study (ECASS) III trial¹¹. The inclusion criteria were as follows : 1) occlusion of the distal intracranial carotid artery (ICA), middle cerebral artery (MCA, M1, or M2), or posterior circulation (vertebral artery, or basilar artery) established by computed tomography angiography (CTA); 2) neurologic deficits; and 3) Solumbra technique thrombectomy with 4 mm Solitaire stent retriever. The exclusion criteria were : 1) the detection of hemorrhage on the initial CT scan; 2) presence of a large ischemic core with an Alberta Stroke Program Early CT Score (ASPECTS) ≤6; 3) MT with a simple stent retriever or the contact aspiration technique. and (4) Solumbra technique thrombectomy with a stent retriever other than a 4 mm Solitaire stent retriever, such as a Solitaire FR 6×30 mm, a Solitaire Platinum 6×40 mm, a Trevo XP Provue (Stryker Neurovascular, Fremont, CA, USA), Eric (MicroVention Terumo, Tustin, CA, USA), or Revive (Codman Neurovascular, San Jose, CA, USA) devices. All patients underwent CT immediately after the intervention to evaluate hemorrhage. In addition, vessel status and hemorrhage were evaluated by CTA 24 hours after MT. Hemorrhagic transformation of the infarct and vessel status was confirmed by magnetic resonance angiography (MRA) with susceptibility-weighted imaging on day 7 after MT.

Device selection and Solumbra technique

Solumbra technique thrombectomy with a 4 mm Solitaire stent retriever was performed in patients with AIS caused by LAO. All of the MT procedures were performed using the Solumbra technique, entailing thrombus retraction with a stent

retriever, such as the Solitaire FR 4×20 mm (ev3; Covidien) or the Solitaire Platinum 4×20 mm or 4×40 mm (Medtronic) and simultaneous aspiration with a 5 Fr SOFIA (Sofia 5; Microvention-Terumo, Tustin, CA, USA) or a 6 Fr AXS Catalyst 6 (CAT6; Stryker Neurovascular, Mountain View, CA, USA). In almost cases, an 8 Fr balloon-guiding catheter (BGC) (FlowGate2 [FG2]; Stryker Neurovascular, Fremont) was ap-

plied. An illustration of MT with the Solumbra technique is shown in (Fig. 1). Under consciousness sedation, an 8 Fr FG2 BGC was placed in the proximal ICA. A microcatheter (Excelsior XT-18; Stryker Neurovascular, Fremont) with a microwire was advanced as distally as possible from the occlusion site, and the aspiration catheter was approached close to the occlusion site, followed by deployment of the stent retriever in the

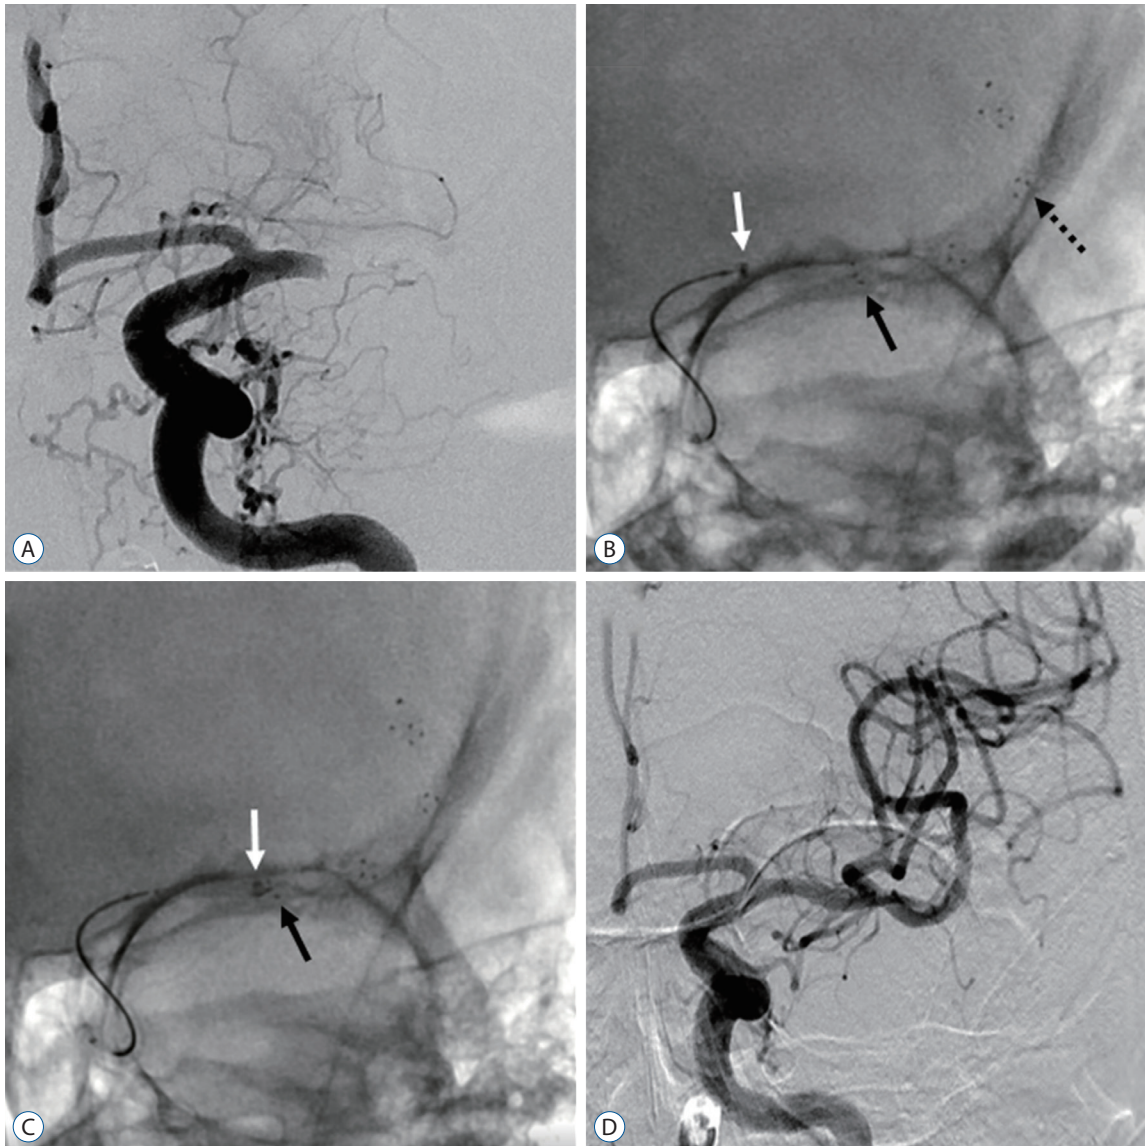


Fig. 1. Solumbra technique thrombectomy with a Solitaire platinum 4×40 mm stent retriever. A : Initial angiography revealed left M1 occlusion. B : A non-subtracted image showed a deployed Solitaire platinum 4×40 mm stent retriever (black arrow : the proximal end of the working device; black dotted arrow : the distal end of the working device) and a 6 French Catalyst (CAT6) aspiration catheter (white arrow : distal tip of the aspiration catheter). C : Using a weak pull of the Solitaire platinum 4×40 mm stent retriever, the distal tip of the CAT6 aspiration catheter is moved to the proximal end of the working length of the stent retriever. To contact the thrombus, the distal tip of the CAT6 should be placed just proximal to the thrombus (black arrow : the proximal end of the working length of the stent; white arrow : distal tip of the aspiration catheter). D : After retrieval of the Solitaire platinum 4×40 mm and CAT6 with simultaneous aspiration, angiography revealed the complete reperfusion status of the left M1.

distal portion of the occlusion site. After the 3 to 5 minutes of waiting after stent deployment to promote stent clot integration³²⁾, the aspiration catheter with suction and the stent retriever were slowly removed as a single unit. At this time, a dual aspiration technique was used at the BGC with manual aspiration¹⁵⁾.

Multivariable factors and outcome and complications

Multivariable factors including patient sex, age, risk factors, prior stroke or transient ischemic attack (TIA), history of previous anti-platelet or anti-coagulant use, ASPECTS score, application of IV t-PA, stroke etiology by Trial of ORG 10172 in Acute Stroke Treatment (TOAST) classification¹⁾, site of the arterial occlusion, and procedure time (time from groin puncture to reperfusion) were reviewed. All patients underwent clinical assessment using the National Institutes of Health Stroke Scale (NIHSS) (range, 0–42; with higher scores indicating more severe neurologic deficit) and modified Rankin Scale (mRS) scores at 3 months (a favorable clinical outcome was defined as mRS ≤2). The radiologic results were evaluated according to the thrombolysis in cerebral infarction (TICI) grading system, successful recanalization (TICI grade of 2b or 3), first-pass reperfusion (modified TICI, mTICI 2b or 3 with the first pass), and first-pass complete reperfusion (mTICI 3 with the first pass). Various complications, such as post-thrombectomy hemorrhage at 24 hours, symptom-related hemorrhage at 24 hours, vessel perforation, arterial dissection, distal emboli, hemorrhagic transformation of the infarct on MRA 7 days after MT, and 3-month mortality were reviewed. Post-thrombectomy hemorrhage at 24 hours was defined as the occurrence of intracerebral hemorrhage or subarachnoid hemorrhage on a CTA scan obtained 24 hours after the procedure. All multimodal factors and clinical data were analyzed by all authors.

Statistical analyses

All data were analyzed using Stata Statistical Software, release 15 (Stata, College Station, TX, USA). Between-group comparisons were calculated using Student's t-test/Mann-Whitney U test or chi-squared test/Fisher's exact test. Multivariate logistic regression analyses were performed for variables with <0.2 level of significance in univariate analysis. Two-tailed *p*-value of ≤0.05 were considered to indicate significant difference.

Table 1. Baseline characteristics of patients in Solumbra technique thrombectomy, according to the length of Solitaire stent retriever

Variable	4x40 (25 patients)	4x20 (45 patients)	<i>p</i> -value*
Dermographic			
Sex, male	14 (56.0)	27 (60.0)	0.601
Age (years)	72.0±12.7	69.0±13.1	0.449
HTN	15 (60.0)	25 (55.6)	0.552
DM	5 (20.0)	10 (22.2)	0.680
Af	8 (32.0)	12 (26.7)	0.346
CAD	5 (20.0)	9 (20.0)	0.889
Dyslipidemia	7 (28.0)	16 (35.6)	0.465
Smoking	5 (20.0)	13 (28.9)	0.263
Prior stroke or TIA	4 (16.0)	7 (15.6)	0.793
Previous anti-platelet use	6 (24.0)	9 (20.0)	0.571
Previous anti-coagulant use	3 (12.0)	4 (8.9)	0.466
Occlusions in the left hemisphere	14 (56.0)	24 (53.3)	0.702
IV t-PA	8 (32.0)	18 (40.0)	0.109
Initial NIHSS	10 (2–18)	8 (2–18)	0.127
ASPECTS score	9 (6–10)	9 (6–10)	0.924
Etiology of stroke			
Cardio-embolic	10 (40.0)	22 (48.9)	0.297
Atherosclerosis	7 (28.0)	10 (22.2)	0.382
Dissection	1 (4.0)	1 (2.2)	0.307
Other or undetermined	7 (28.0)	12 (26.7)	0.693
Site of arterial occlusion			
MCA	13 (52.0)	27 (60.0)	0.419
Distal ICA	10 (40.0)	13 (28.9)	0.310
Posterior circulation	2 (8.0)	5 (11.1)	0.507
Procedure detail			
Procedure time (minutes)	34 (14–82)	46 (15–91)	0.247
Use of BGC	24 (96.0)	42 (93.3)	0.776
Aspiration catheter, CAT6:Sofia5	21 : 4	33 : 12	0.186
Radiopaque stent retriever	25 (100.0)	20 (44.4)	0.001 [†]

Values are presented as mean±standard deviation, median (interquartile range), or number (%). **p*-values are calculated by chi-square test or Fisher's exact test and Mann-Whitney U test or Student's t-test. [†]Statistically significant. 4x40 : Solitaire Platinum 4x40 mm stent retriever, 4x20 : Solitaire 2 FR 4x20 mm stent retriever + Solitaire Platinum 4x20 mm stent retriever, HTN : hypertension, DM : diabetes mellitus, Af : atrial fibrillation, CAD : coronary artery disease, TIA : transient ischemic attack, IV t-PA : intravenous tissue-plasminogen activator, NIHSS : National Institutes of Health Stroke Scale, ASPECT : Alberta Stroke Program Early CT, MCA : middle cerebral artery, ICA : internal carotid artery, BGC : balloon guide catheter, CAT6 : 6 Fr Catalyst, Sofia5 : 5 Fr Sofia

RESULTS

Baseline characteristics and procedure detail

Twenty-five patients (14 males, 56.0%) were treated via Solumbra technique thrombectomy with 4×40 mm Solitaire Platinum stent retriever (4×40 group), and 45 (27 males, 60.0%) underwent Solumbra technique thrombectomies with 4×20 mm Solitaire stent retrievers (4×20 group). The mean age of the patients in the 4×40 group was 72 years (standard deviation [SD], 12.7) and that of the 4×20 group was 69 years (SD, 13.1). There were no significant differences in multiple risk factors such as hypertension, diabetes mellitus, atrial fibrillation, coronary artery disease, dyslipidemia, smoking, history of prior stroke or TIA, history of anti-platelet use, previous anti-coagulation use, the proportion of left hemisphere strokes, and the rate of IV t-PA application, between 4×40 and

4×20 groups. The median initial NIHSS value, and ASPECTS scores were 10 and 9, respectively, in the 4×40 group and 8 and 9, respectively, in the 4×20 group, without significant difference. There was no significant difference in stroke etiology between the two groups. The site of arterial occlusion in each group was as follows (4×40 group : 4×20 group) : MCA, 13 : 27; distal ICA, 10 : 13; and posterior circulation, 2 : 5. In terms of procedure, there were no statistically significant differences in procedure time and the rate of BGC application between the two groups ($p=0.247$ and 0.776 , respectively). The distribution ratio of the two-aspiration catheters (CAT6 : Sofia5) was 21 : 4 in the 4×40 group, and 33 : 12 in the 4×20 group ($p=0.186$). Radiopaque devices were significantly more common in the 4×40 group ($p=0.001$), suggesting that 25 non-radiopaque Solitaire FR 4×20 mm stents were included in the 4×20 group (Table 1).

Table 2. Outcomes and complications of patients in Solumbra technique thrombectomy, according to the length of Solitaire stent retriever

	4×40 (25 patients)	4×20 (45 patients)	<i>p</i> -value*
Outcome			
Successful recanalization	24 (96.0)	43 (95.6)	0.842
First-pass reperfusion	17 (68.0)	21 (46.7)	0.004 [†]
First-pass complete reperfusion	12 (48.0)	15 (33.3)	0.007 [†]
Favorable 3 months mRS	14 (56.0)	23 (51.1)	0.592
Complication			
Post thrombectomy hemorrhage	2 (8.0)	4 (8.9)	0.627
Symptomatic hemorrhage	1 (4.0)	2 (4.4)	0.793
Vessel perforation	0 (0.0)	0 (0.0)	1.000
Arterial dissection	0 (0.0)	0 (0.0)	1.000
Distal emboli	2 (8.0)	4 (8.9)	0.679
Hemorrhagic transformation of infarct	4 (16.0)	9 (20.0)	0.391
3 months mortality	2 (8.0)	4 (8.9)	0.497

Values are presented as number (%). **p*-values are calculated by chi-square test or Fisher's exact test and Mann-Whitney U test or Student's *t*-test. [†]Statistically significant. 4×40 : Solitaire Platinum 4×40 mm stent retriever, 4×20 : Solitaire 2 FR 4×20 mm stent retriever + Solitaire Platinum 4×20 mm stent retriever, Successful recanalization : thrombolysis in cerebral infarction 2b or 3, mRS : modified Rankin Scale, Favorable mRS : 90 days mRS ≤2, First-pass reperfusion : modified thrombolysis in cerebral infarction 2b or 3 with the first pass, First-pass complete reperfusion : modified thrombolysis in cerebral infarction 3 with the first pass

Outcomes and complications

No statistically significant difference was found in the rate of successful recanalization, between the two groups (4×40 group : 4×20 group, 96.0% : 95.6%; $p=0.842$). However, the

Table 3. Multivariable regression for first-pass reperfusion and first-pass TIC3 reperfusion

	OR	95% CI	<i>p</i> -value*
First-pass reperfusion			
Initial NIHSS	2.95	0.61–4.38	0.442
IV t-PA	0.97	0.58–2.26	0.367
CAT6 Aspiration catheter	1.86	0.78–3.14	0.172
Radiopaque stent retriever	2.08	1.22–3.84	0.014 [†]
Long stent retriever (Platinum 4×40 mm)	2.81	1.34–4.10	0.008 [†]
First-pass complete reperfusion			
Initial NIHSS	2.72	0.58–4.46	0.407
IV t-PA	0.82	0.66–3.08	0.266
CAT6 Aspiration catheter	2.06	0.82–3.90	0.312
Radiopaque stent retriever	1.88	1.20–3.12	0.022 [†]
Long stent retriever (Platinum 4×40 mm)	2.12	1.48–3.76	0.012 [†]

**p*-values are calculated by multivariate logistic regression analysis. [†]Statistically significant. TIC1 : thrombolysis in cerebral infarction, OR : odds ratio, CI : confidence interval, First-pass reperfusion : modified TIC1 2b or 3 with the first pass, NIHSS : National Institutes of Health Stroke Scale, IV t-PA : intravenous tissue-plasminogen activator, CAT6 : 6 French Catalyst, First-pass complete reperfusion : modified TIC1 3 with the first pass

proportion of first-pass reperfusions and first-pass complete reperfusions was significantly higher in the 4×40 group, compared to the 4×20 group (68.0% vs. 46.7% and 48.0% vs. 33.3%, $p=0.004$ and 0.007 , respectively). There were no significant differences in complications, between the two groups (Table 2).

Predictors of reperfusion and full reperfusion with first pass

In multivariate logistic regression analysis, the use of radiopaque Solitaire stent retriever (odds ratio [OR], 2.08; 95% confidence interval [CI], 1.22–3.84; $p=0.014$), and longer Solitaire Platinum 4×40 mm stent retrievers (OR, 2.81; 95% CI, 1.34–4.10; $p=0.008$) were correlated with first-pass reperfusion. In addition, multivariate logistic regression analysis for first-pass complete reperfusion indicated that the use of radiopaque devices (OR, 1.88; 95% CI, 1.20–3.12; $p=0.022$) and longer Solitaire Platinum 4×40 mm stents (OR, 2.12; 95% CI, 1.48–3.76; $p=0.012$) were independent predictors (Table 3).

DISCUSSION

Currently, the development of various thrombectomy tech-

niques has enhanced the clinical and radiologic outcomes of patients with LAO^{6,7,19}. Recent advances in MT pursuit the first pass effect (first-pass reperfusion or first-pass complete reperfusion), beyond simple successful recanalization²⁵. The importance of the first-pass effect has been reported in various studies, where it was associated with a significantly higher chance of favorable clinical outcomes with the retrieval of the entire thrombus as a single mass on the first attempt^{23,24,34}. Fewer stent passages reduced the risk of procedure-related complications, such as parenchymal hematoma and other vessel damage³. Therefore, the utility of the Solumbra technique contributes to reperfusion or complete reperfusion from the first pass^{14,21,25}. Based on these studies, the authors used Solumbra technique for MT in most cases. In addition to thrombectomy techniques, the device may be considered a factor affecting the outcomes of MT. There are several controversies related to the selective advantages of stent retrievers with an appropriate diameter. However, recent studies have suggested that stent retrievers with longer lengths and radiopaque characteristics yield better outcomes^{12,13,18,31}. In our study, longer and radiopaque stent retrievers were found to increase the first-pass effect. The reperfusion and complete reperfusion rates with first pass were significantly higher in the group with 4×40 mm long stent retrievers than in those with 4×20 mm

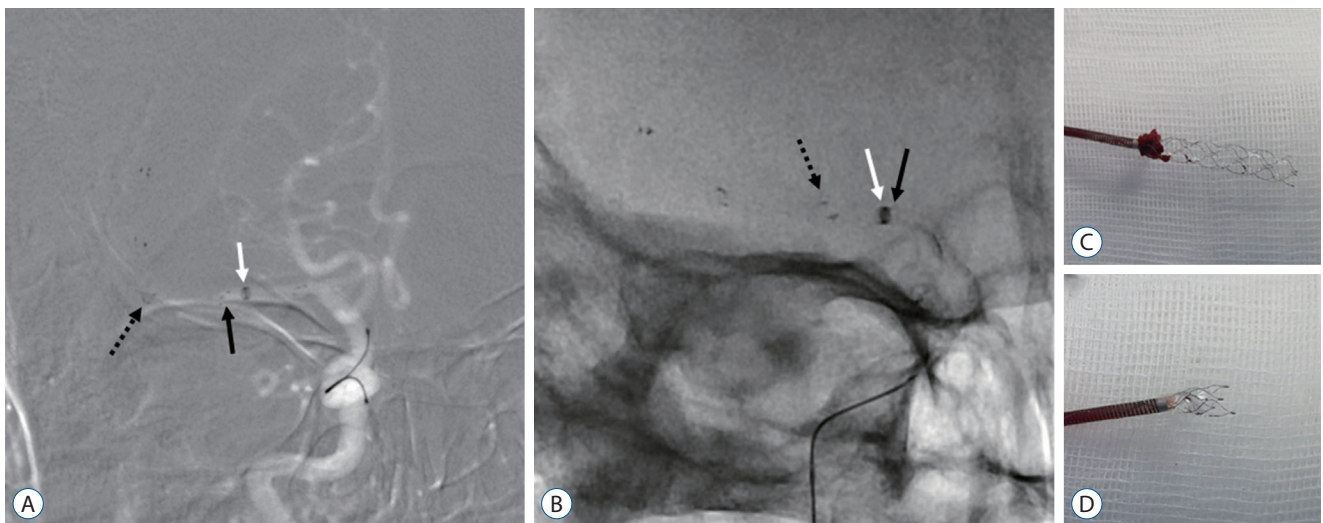


Fig. 2. Representative case of solumbra technique thrombectomy with a Solitaire platinum 4×40 mm stent retriever. A : Roadmap image shows the location of the devices, before their retrieval (black arrow : the proximal end of the working length of the stent; black dotted arrow : mid-portion marker of the stent; white arrow : distal tip of the aspiration catheter). B : By a weak pull of the Solitaire platinum 4×40 mm stent retriever, the distal tip of aspiration catheter (white arrow) should be placed just proximal to the thrombus and between the two markers (black and black dotted arrows) of the Solitaire platinum 4×40 mm stent. C : After retrieval of the Solumbra technique devices, the thrombus was captured by the aspiration catheter and stent retriever. D : Image of the solumbra technique system after retrieval, in which the tip of the aspiration catheter was located distally beyond the mid-portion marker of the stent retriever.

short stent retrievers. Furthermore, the multivariate analysis in our study showed that stent retrievers with longer length and radiopacity improved the first-pass effect in MT with Solumbra technique. These findings revealed the effectiveness of Solitaire Platinum 4×40 mm stent retrievers compared to other 4 mm Solitaire stent retrievers, especially in MT with the Solumbra technique.

Longer stent retrievers have theoretical advantages because of the larger interaction area between the device and the thrombus, with lower chances of missing the target site than their shorter counterparts. In addition, the radiopaque characteristics of the device allow the interventionalists to view the entire stent, and confirm its optimal location and adequate vessel-wall apposition of the stent. Based on these characteristics, the usefulness of the Solitaire Platinum 4×40 mm stent retriever and its technical considerations during the Solumbra technique thrombectomy was shown in (Fig. 2). Under road-map guidance, the microcatheter was navigated distal to the occlusion site, and the Solitaire Platinum 4×40 mm stent retriever was deployed to cover the distal and proximal ends of the occlusion. The aspiration catheter was navigated close to the clot, and the microcatheter was removed to increase the aspiration flow (Fig. 2A)²⁶. Next, the stent retriever was gently pulled with weak force and the distal tip of the aspiration catheter was moved to the distal lesion as close to the occlusion site as possible to contact the thrombus. At this time, the distal tip of the aspiration catheter should be placed just proximal to the site of the thrombus, between the two markers (mid-portion of the marker and the proximal end of the working length marker) of the Solitaire platinum 4×40 mm stent retriever (Fig. 2B). After waiting several minutes to enable stent-clot integration, retrieval of the whole Solumbra system was performed for clot retrieval, with simultaneous continuous suction at the aspiration catheter and dual aspiration through the BGC. When the distal tip of the aspiration catheter was adequately positioned between the mid-portion marker and the proximal end of the working length marker without crossing the mid-portion marker, the thrombus could be retrieved as a single mass (Fig. 2C). However, frequent failures associated with thrombus retrieval occurred when the distal tip of the aspiration catheter was located more distally, beyond the mid-portion of the stent, and re-captured more than half of the stent retriever (Fig. 2D).

In the thrombectomy procedures using the Solumbra tech-

nique, the aspiration catheter should re-capture less than half or one-third of the stent retriever to ensure an adequate stent retriever capture area to fully integrate with the clot. In addition, during the Solumbra system retrieval, the aspiration catheter is moved further distally depending on its tension, and the stent retriever is captured further by the aspiration catheter. In addition to the advantage of a long stent, the radiopacity of the Solitaire Platinum 4×40 mm stent retriever with its markers 10 mm apart facilitate the correct positioning of the aspiration catheter and adjust the adequate capture range of the stent retrievers, especially during Solumbra technique thrombectomy. Therefore, a long and radiopaque stent retriever such as the Solitaire Platinum 4×40 mm stent retriever, is preferred for MT by Solumbra technique.

The major limitations of this study were its relatively small sample size, and the retrospective non-blinded format. Since thrombectomy in the 4×20 mm Solitaire stent retriever group was performed earlier than in the 4×40 mm Solitaire Platinum stent retriever group, it may be assumed that the learning curve affected the outcome. However, all thrombectomy procedures in this study were performed by neuro-interventionalists with several years of experience. Therefore, the learning curve would not have a significant influence on the outcome. Furthermore, the baseline characteristics in the two groups were well balanced and there were no statistically significant differences. The disadvantages of longer stent retrievers include vessel damage or larger interface area with the vessel and consequently more friction. However, in our study, there were no significant differences in hemorrhage and dissection between the two groups. In addition, our study did not include the data associated with Solitaire FR 4×40 mm retriever, which is a non-radiopaque and long Solitaire stent retriever. Other potential unmeasured confounding variables were not controlled for, although every effort was made to adjust for the possibility of spurious results.

CONCLUSION

In this study, the use of the Solitaire Platinum 4×40 mm stent retriever for Solumbra technique thrombectomy in patients with LAO was highly effective, without increased periprocedural complications, compared with prior versions of the Solitaire FR 4×20 mm stent and the Solitaire Platinum 4×

20 mm stent. The radiopacity and long length of the Solitaire Platinum 4×40 mm stent retriever may contribute to more achievement of first-pass reperfusion and first-pass complete reperfusion, especially with Solumbra technique thrombectomy. Future prospective multicenter and *in vitro* studies are needed to corroborate our findings.

CONFLICTS OF INTEREST

No potential conflict of interest relevant to this article was reported.

INFORMED CONSENT

This type of study does not require informed consent.

AUTHOR CONTRIBUTIONS

Conceptualization : HJY, JHS

Data curation : HJY

Formal analysis : HJY

Methodology : HJY

Project administration : HJY, JHS

Visualization : HJY

Writing - original draft : HJY

Writing - review & editing : HJY, JHS, DHL, SYS

ORCID

Ho Jun Yi <https://orcid.org/0000-0003-3061-0689>
 Jae Hoon Sung <https://orcid.org/0000-0003-3738-6413>
 Dong Hoon Lee <https://orcid.org/0000-0002-3796-8707>
 Seung Yoon Song <https://orcid.org/0000-0002-6120-2795>

References

- Amarenco P, Bogousslavsky J, Caplan LR, Donnan GA, Hennerici MG : Classification of stroke subtypes. **Cerebrovasc Dis** **27** : 493-501, 2009
- Berkhemer OA, Fransen PS, Beumer D, van den Berg LA, Lingsma HF, Yoo AJ, et al. : A randomized trial of intraarterial treatment for acute ischemic stroke. **N Engl J Med** **372** : 11-20, 2015
- Bourcier R, Saleme S, Labreuche J, Mazighi M, Fahed R, Blanc R, et al. : More than three passes of stent retriever is an independent predictor of parenchymal hematoma in acute ischemic stroke. **J Neurointerv Surg** **11** : 625-629, 2019
- Bracard S, Ducrocq X, Mas JL, Soudant M, Oppenheim C, Moulin T, et al. : Mechanical thrombectomy after intravenous alteplase versus alteplase alone after stroke (THRACE): a randomised controlled trial. **Lancet Neurol** **15** : 1138-1147, 2016
- Campbell BC, Mitchell PJ, Kleinig TJ, Dewey HM, Churilov L, Yassi N, et al. : Endovascular therapy for ischemic stroke with perfusion-imaging selection. **N Engl J Med** **372** : 1009-1018, 2015
- Dargazanli C, Consoli A, Barral M, Labreuche J, Redjem H, Ciccio G, et al. : Impact of modified TIC1 3 versus modified TIC1 2b reperfusion score to predict good outcome following endovascular therapy. **AJNR Am J Neuroradiol** **38** : 90-96, 2017
- Dargazanli C, Fahed R, Blanc R, Gory B, Labreuche J, Duhamel A, et al. : Modified thrombolysis in cerebral infarction 2C/thrombolysis in cerebral infarction 3 reperfusion should be the aim of mechanical thrombectomy: insights from the ASTER trial (contact aspiration versus stent retriever for successful revascularization). **Stroke** **49** : 1189-1196, 2018
- Dashaies EM : Tri-axial system using the Solitaire-FR and Penumbra Aspiration Microcatheter for acute mechanical thrombectomy. **J Clin Neurosci** **20** : 1303-1305, 2013
- Goyal M, Demchuk AM, Menon BK, Eesa M, Rempel JL, Thornton J, et al. : Randomized assessment of rapid endovascular treatment of ischemic stroke. **N Engl J Med** **372** : 1019-1030, 2015
- Goyal M, Menon BK, van Zwam WH, Dippel DW, Mitchell PJ, Demchuk AM, et al. : Endovascular thrombectomy after large-vessel ischaemic stroke: a meta-analysis of individual patient data from five randomised trials. **Lancet** **387** : 1723-1731, 2016
- Hacke W, Kaste M, Bluhmki E, Brozman M, Dávalos A, Guidetti D, et al. : Thrombolysis with alteplase 3 to 4.5 hours after acute ischemic stroke. **N Engl J Med** **359** : 1317-1329, 2008
- Haussen DC, Al-Bayati AR, Grossberg JA, Bouslama M, Barreira C, Bianchi N, et al. : Longer stent retrievers enhance thrombectomy performance in acute stroke. **J Neurointerv Surg** **11** : 6-8, 2019
- Haussen DC, Lima A, Nogueira RG : The Trevo XP 3×20 mm retriever ('Baby Trevo') for the treatment of distal intracranial occlusions. **J Neurointerv Surg** **8** : 295-299, 2016
- Hesse AC, Behme D, Kemmling A, Zapf A, Große Hokamp N, Frischmuth I, et al. : Comparing different thrombectomy techniques in five large-volume centers: a 'real world' observational study. **J Neurointerv Surg** **10** : 525-529, 2018
- Hopf-Jensen S, Preiß M, Marques L, Lehrke S, Schattschneider J, Stolze H, et al. : Impact and effectiveness of dual aspiration technique in stent-assisted mechanical thrombectomy: recent improvements in acute stroke management. **Cardiovasc Intervent Radiol** **39** : 1620-1628, 2016
- Humphries W, Hoit D, Doss VT, Elijovich L, Frei D, Loy D, et al. : Distal aspiration with retrievable stent assisted thrombectomy for the treatment of acute ischemic stroke. **J Neurointerv Surg** **7** : 90-94, 2015

17. Jovin TG, Chamorro A, Cobo E, de Miquel MA, Molina CA, Rovira A, et al. : Thrombectomy within 8 hours after symptom onset in ischemic stroke. **N Engl J Med** 372 : 2296-2306, 2015
18. Kabbasch C, Mpotsaris A, Chang DH, Hiß S, Dorn F, Behme D, et al. : Mechanical thrombectomy with the Trevo ProVue device in ischemic stroke patients: does improved visibility translate into a clinical benefit? **J Neurointerv Surg** 8 : 778-782, 2016
19. Kaesmacher J, Maegerlein C, Zibold F, Wunderlich S, Zimmer C, Friedrich B : Improving mTICI2b reperfusion to mTICI2c/3 reperfusions: a retrospective observational study assessing technical feasibility, safety and clinical efficacy. **Eur Radiol** 28 : 274-282, 2018
20. Kang DH, Kim YW, Hwang YH, Park J, Hwang JH, Kim YS : Switching strategy for mechanical thrombectomy of acute large vessel occlusion in the anterior circulation. **Stroke** 44 : 3577-3579, 2013
21. Maegerlein C, Berndt MT, Mönch S, Kreiser K, Boeckh-Behrens T, Lehm M, et al. : Further development of combined techniques using stent retrievers, aspiration catheters and BGC : the PROTECTPLUS technique. **Clin Neuroradiol** 30 : 59-65, 2020
22. Maegerlein C, Mönch S, Boeckh-Behrens T, Lehm M, Hedderich DM, Berndt MT, et al. : PROTECT: PProximal balloon Occlusion TogEther with direCt Thrombus aspiration during stent retriever thrombectomy - evaluation of a double embolic protection approach in endovascular stroke treatment. **J Neurointerv Surg** 10 : 751-755, 2018
23. Maus V, Behme D, Kabbasch C, Borggrefe J, Tsogkas I, Nikoubashman O, et al. : Maximizing first-pass complete reperfusion with SAVE. **Clin Neuroradiol** 28 : 327-338, 2018
24. Maus V, Brehm A, Tsogkas I, Henkel S, Psychogios MN : Stent retriever placement in embolectomy: the choice of the post-bifurcational trunk influences the first-pass reperfusion result in M1 occlusions. **J Neurointerv Surg** 11 : 237-240, 2019
25. Mizokami T, Uwatoko T, Matsumoto K, Ooya Y, Hashimoto G, Koguchi M, et al. : Aspiration Catheter Reach to Thrombus (ART) sign in combined technique for mechanical thrombectomy: impact for first-pass complete reperfusion. **J Stroke Cerebrovasc Dis** 28 : 104301, 2019
26. Nikoubashman O, Alt JP, Nikoubashman A, Büsen M, Heringer S, Brockmann C, et al. : Optimizing endovascular stroke treatment: removing the microcatheter before clot retrieval with stent-retrievers increases aspiration flow. **J Neurointerv Surg** 9 : 459-462, 2017
27. Pérez MA, Miloslavski E, Fischer S, Bänzner H, Henkes H : Intracranial thrombectomy using the Solitaire stent: a historical vignette. **J Neurointerv Surg** 4 : e32, 2012
28. Pfaff J, Rohde S, Engelhorn T, Doerfler A, Bendszus M, Möhlenbruch MA : Mechanical thrombectomy using the new Solitaire™ Platinum stent-retriever : reperfusion results, complication rates and early neurological outcom. **Clin Neuroradiol** 29 : 311-319, 2019
29. Saver JL, Goyal M, Bonafe A, Diener HC, Levy EI, Pereira VM, et al. : Stent-retriever thrombectomy after intravenous t-PA vs. t-PA alone in stroke. **N Engl J Med** 372 : 2285-2295, 2015
30. Turk AS, Frei D, Fiorella D, Mocco J, Baxter B, Siddiqui A, et al. : ADAPT FAST study: a direct aspiration first pass technique for acute stroke thrombectomy. **J Neurointerv Surg** 6 : 260-264, 2014
31. Yang D, Hao Y, Zi W, Wang H, Zheng D, Li H, et al. : Effect of retrievable stent size on endovascular treatment of acute ischemic stroke: a multi-center study. **AJNR Am J Neuroradiol** 38 : 1586-1593, 2017
32. Yi HJ, Lee DH, Sung JH : Clinical usefulness of waiting after stent deployment in mechanical thrombectomy: effect of the clot integration. **World Neurosurg** 119 : e87-e93, 2018
33. Yi HJ, Sung JH, Lee DH, Hong JT, Lee SW : Single-center experience of mechanical thrombectomy with the Trevo XP ProVue 6 × 25 mm stent retriever in middle cerebral artery occlusion: comparison with Trevo XP ProVue 4 × 20 mm. **World Neurosurg** 107 : 649-656, 2017
34. Zaidat OO, Castonguay AC, Linfante I, Gupta R, Martin CO, Holloway WE, et al. : First pass effect: a new measure for stroke thrombectomy devices. **Stroke** 49 : 660-666, 2018